



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4945 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # 01923080A3 Cyl. # 55)
Keys Yes or No
Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: BMDC
5. Battery Check
Was the external battery pack replaced? Yes or No
6. O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 250 psi Regulator: 300 psi
Display and Regulator \pm 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value \leq 0.03 AC: 0.020 AC
Sim. Ser #: MP3002
Lot #: 202301E
Exp. Date: 17Jan 25
 Results \pm 0.005 of known AC

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP6636
 Lot #: 202212C
 Exp. Date: 08Dec24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 14323080A4
 Cylinder #: 43
 Exp. Date: 015/25
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7344
 Lot #: ICS 8
 Exp. Date: NIA
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)


Test 1	<u>0.080</u>	Test 4	<u>0.081</u>	Test 7	<u>0.081</u>
Test 2	<u>0.081</u>	Test 5	<u>0.081</u>	Test 8	<u>0.081</u>
Test 3	<u>0.081</u>	Test 6	<u>0.081</u>	Test 9	<u>0.081</u>
Average <u>0.080</u>					

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No
 If No, state reason(s) why: _____

If Yes, change location code back to A.4.

<u></u>	<u>16 Apr 2024</u>
Inspector Signature	Date
<u>Janelle Putscheller</u>	<u>18 Apr 2024</u>
Reviewer	Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:13

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01923080A3
Standard Cyl #? 55
Standard Expiration? 02/05/2025
Oper No? 133237

Flow Cal. Date: 09/26/2012
Slope 622
Intercept -485836

IR Calibration Date: 04/22/2016
 3um 9um

0th Coef(*100): -23427 -26406
1st Coef(*100): 266989 144341
2nd Coef(*100): 2085 1078
H2O adj(mg/l*10k): 539 400

***** Printer Test End *****

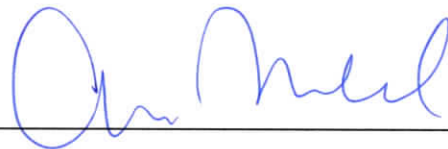

Operator Signature
ANNA NAREHOOD

Remarks: *Print Test*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:14

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:14
02 Std. Sol.	0.019	10:15
03 Room Air	0.000	10:16
04 Std. Sol.	0.020	10:16
05 Room Air	0.000	10:17
06 Std. Sol.	0.020	10:18
07 Room Air	0.000	10:18

08 Sim Temp = 34.0°C

Simul Ser No = MP3002
Std Sol No = 202301E
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *LOW AC check - 0.020AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:19

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:20
02 Std. Sol.	0.399	10:20
03 Room Air	0.000	10:21
04 Std. Sol.	0.402	10:22
05 Room Air	0.000	10:22
06 Std. Sol.	0.402	10:23
07 Room Air	0.000	10:24


08 Sim Temp = 34.0°C

Simul Ser No = MP6036

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Day cal check - 0.400AC*
Wet high AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:25

Test	AC	Time
01 Room Air	0.000	10:25
02 *Subject Test	INT*	10:26
03 Room Air	0.000	10:27

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 43
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:27

Test	AC	Time
01 Diagnostic	OK	10:28
02 Room Air	0.000	10:28
03 *Subject Test	RFI*	10:29
04 Room Air	0.000	10:29

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 43
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: *RFI check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:29

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:30
02 Std. Gas	0.080	10:30
03 Room Air	0.000	10:31
04 Std. Gas	0.081	10:31
05 Room Air	0.000	10:32
06 Std. Gas	0.081	10:32
07 Room Air	0.000	10:33

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:34

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:34
02 Std. Gas	0.081	10:35
03 Room Air	0.000	10:35
04 Std. Gas	0.081	10:36
05 Room Air	0.000	10:36
06 Std. Gas	0.081	10:36
07 Room Air	0.000	10:37

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

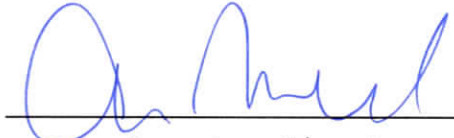
Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-4

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = TOXL 8164.14.00 09/16
04/16/2024 10:38

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:39
02 Std. Gas	0.081	10:39
03 Room Air	0.000	10:40
04 Std. Gas	0.081	10:40
05 Room Air	0.000	10:40
06 Std. Gas	0.081	10:41
07 Room Air	0.000	10:41

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000