



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 5938 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # _____ Cyl. # _____)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data Unable to connect
3. Upload Operator File
4. Current Location Code: TOXL
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 395 psi Regulator: 500 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: 411 psi Regulator: 450 psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3002
Lot #: 2023DIE
Exp. Date: 17Jan25
 Results ± 0.005 of known AC

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP6036
 Lot #: 202212C
 Exp. Date: 08 Dec 24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 14323080A4
 Cylinder #: 43
 Exp. Date: 015125
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7344
 Lot #: ICS 8
 Exp. Date: NIA
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)

Test 1	<u>0.079</u>	Test 4	<u>0.080</u>	Test 7	<u>0.081</u>
Test 2	<u>0.080</u>	Test 5	<u>0.080</u>	Test 8	<u>0.080</u>
Test 3	<u>0.081</u>	Test 6	<u>0.080</u>	Test 9	<u>0.080</u>
		Average	<u>0.080</u>		

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No
 If No, state reason(s) why: unable to direct connect to instrument to upload operator file.

If Yes, change location code back to A.4.

[Signature]
 Inspector Signature

16 Apr 2024
 Date

[Signature]
 Reviewer

18 Apr 2024
 Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:06

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 26021080A1
Standard Cyl #? 3
Standard Expiration? 10/05/2023
Oper No? 133237

Flow Cal. Date: 07/15/2013
Slope 664
Intercept -578364

IR Calibration Date: 07/27/2015
 3um 9um

0th Coef(*100): -14232 -19463
1st Coef(*100): 289698 139293
2nd Coef(*100): 2380 1071
H2O adj(mg/l*10k): 253 294

***** Printer Test End *****

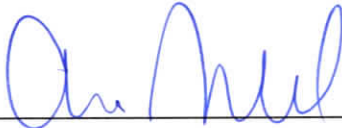

Operator Signature
ANNA NAREHOOD

Remarks: Pmt Test

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:07

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:08
02 Std. Sol.	0.020	09:09
03 Room Air	0.000	09:09
04 Std. Sol.	0.021	09:10
05 Room Air	0.000	09:10
06 Std. Sol.	0.021	09:11
07 Room Air	0.000	09:12


08 Sim Temp = 34.0°C

Simul Ser No = MP3002

Std Sol No = 202301E

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Low Ac Check - 0.020AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:13

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:13
02 Std. Sol.	0.399	09:15
03 Room Air	0.000	09:16
04 Std. Sol.	0.400	09:16
05 Room Air	0.000	09:17
06 Std. Sol.	0.402	09:18
07 Room Air	0.000	09:18


08 Sim Temp = 34.0°C

Simul Ser No = MP6036

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High Ac Check - 0.400AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:19

Test	AC	Time
01 Room Air	0.000	09:20
02 *Subject Test	INT*	09:20
03 Room Air	0.000	09:21

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 13
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:23

Test	AC	Time
01 Diagnostic	OK	09:24
02 Room Air	0.000	09:24
03 *Subject Test	RFI*	09:25
04 Room Air	0.000	09:26

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 43
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:28
02 Std. Gas	0.079	09:29
03 Room Air	0.000	09:29
04 Std. Gas	0.080	09:30
05 Room Air	0.000	09:30
06 Std. Gas	0.081	09:31
07 Room Air	0.000	09:31

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

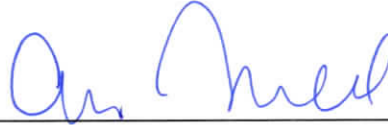

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check - #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:33

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:34
02 Std. Gas	0.080	09:34
03 Room Air	0.000	09:35
04 Std. Gas	0.080	09:35
05 Room Air	0.000	09:35
06 Std. Gas	0.080	09:36
07 Room Air	0.000	09:36

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

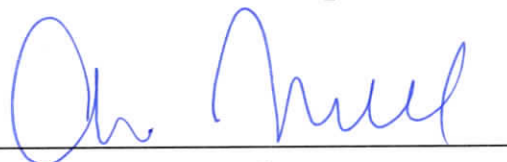

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005938
Location = TOXL 8164.14.00 09/16
04/16/2024 09:38

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:38
02 Std. Gas	0.081	09:39
03 Room Air	0.000	09:39
04 Std. Gas	0.080	09:40
05 Room Air	0.000	09:40
06 Std. Gas	0.080	09:41
07 Room Air	0.000	09:41

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Dry cal check #7-9*

Form 106-I8000