



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 80-004938	Instrument Location Killdeer Police Department
Reason for Install/Repair <input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <u>Annual inspection from Crime Lab</u>	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): _____
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date 4/26/24
-------------------------------	-----------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By 	Certified Date 29April2024
---------------------------	-------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004938
Location = KDPD 8164.14.00 09/16
04/26/2024 13:50

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 14323080A4
Standard Cyl #? 42
Standard Expiration? 06/05/2025
Oper No? 130396

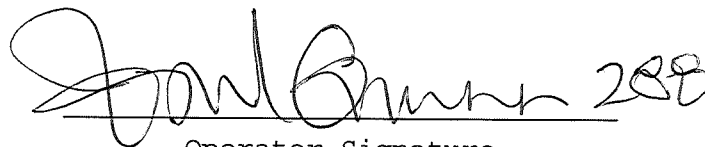
Flow Cal. Date: 06/10/2020
Slope 587
Intercept -338327

IR Calibration Date: 06/10/2020

	3um	9um
--	-----	-----

0th Coef(*100):	-22434	-23179
1st Coef(*100):	269849	136790
2nd Coef(*100):	963	840
H2O adj(mg/l*10k):	355	370

***** Printer Test End *****



Operator Signature
ERIN QUINN

Remarks:

Form 106-I8000

True and Original Form
Date: 4/26/24
Sign: 

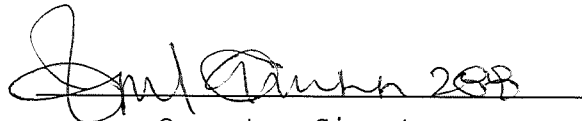
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004938
Location = KDPD 8164.14.00 09/16
04/26/2024 13:51

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:51
02 Std. Gas	0.079	13:52
03 Room Air	0.000	13:52
04 Std. Gas	0.079	13:53
05 Room Air	0.000	13:53
06 Std. Gas	0.080	13:54
07 Room Air	0.000	13:54

Lot No = 14323080A4
Cyl No = 42
Exp Date = 06/05/2025
County = 13 Oper No. = 130396


Operator Signature
ERIN QUINN

Remarks:

Form 106-I8000

True and Original Form
Date: 4/26/24
Sign: 


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004938
Location = KOPD 8164.14.00 09/16
04/26/2024 13:55

Test	AC	Time
01 Room Air	0.000	13:59
02 *Subject Test	RFI*	13:59
03 Room Air	0.000	14:00

*Invalid Test
Inhibited - RFI

Sub Name = RFI TEST, INSTALL NA
Sub DOB = 12/30/1999
Sub Sex = Unknown Weight = NA
Test = OTH Cit = NA
Dr. Lic. = ND/NA
Lot No = 14323080A4
Cyl No = 42
Expiration Date = 06/05/2025
County = 13 Oper No. = 130396


Operator Signature
ERIN QUINN

Remarks:

Form 106-I8000

True and Original Form

Date: 4/26/24
Sign: [Signature]

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004938
Location = KOPD 8164.14.00 09/16
04/26/2024 14:01

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	14:02
02 Room Air	0.000	14:02

*Invalid Test
Inhibited - RFI

Lot No = 14323080A4
Cyl No = 42
Exp Date = 06/05/2025
County = 13 Oper No. = 130396


Operator Signature
ERIN QUINN

Remarks:

True and Original Form

Date: 4/26/24
Sign: [Signature]