



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4936 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 01923080A3 Cyl. # 52)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: BOTT
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 757 psi Regulator: 750 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3002
Lot #: 202301E
Exp. Date: 17Jan25
 Results ± 0.005 of known AC

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP6036
 Lot #: 202212C
 Exp. Date: 08DEC24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 14323080A4
 Cylinder #: 12
 Exp. Date: 015125
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7344
 Lot #: 1CS8
 Exp. Date: N/A
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)

Test 1	<u>0.080</u>	Test 4	<u>0.079</u>	Test 7	<u>0.079</u>
Test 2	<u>0.080</u>	Test 5	<u>0.079</u>	Test 8	<u>0.079</u>
Test 3	<u>0.080</u>	Test 6	<u>0.080</u>	Test 9	<u>0.080</u>
		Average	<u>0.079</u>		

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4. N/A Instrument swapped

[Signature]
 Inspector Signature

29 Apr 2024
 Date

[Signature]
 Reviewer

30 Apr 2024
 Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 11:12

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01923080A3
Standard Cyl #? 52
Standard Expiration? 02/05/2025
Oper No? 133237

Flow Cal. Date: 01/18/2010
Slope 732
Intercept -767769

IR Calibration Date: 04/20/2016
 3um 9um

0th Coef(*100): -15846 -19883
1st Coef(*100): 260423 131703
2nd Coef(*100): 1755 1110
H2O adj(mg/l*10k): 371 394

***** Printer Test End *****



Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 11:57

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:58
02 Std. Sol.	0.021	11:58
03 Room Air	0.000	11:59
04 Std. Sol.	0.021	12:00
05 Room Air	0.000	12:00
06 Std. Sol.	0.022	12:01
07 Room Air	0.000	12:01

08 Sim Temp = 34.0°C

Simul Ser No = MP3002

Std Sol No = 202301E

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Low AC Check - 0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 12:12

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:13
02 Std. Sol.	0.397	12:14
03 Room Air	0.000	12:15
04 Std. Sol.	0.400	12:16
05 Room Air	0.000	12:16
06 Std. Sol.	0.400	12:17
07 Room Air	0.000	12:17


08 Sim Temp = 34.0°C

Simul Ser No = MP6036

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High Ac Check - 0.400Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 12:21

Test	AC	Time
01 Room Air	0.000	12:22
02 *Subject Test	INT*	12:23
03 Room Air	0.000	12:23

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 12
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 12:24

Test	AC	Time
01 Diagnostic	OK	12:25
02 Room Air	0.000	12:25
03 *Subject Test	RFI*	12:25
04 Room Air	0.000	12:26

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 12
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 12:26

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:27
02 Std. Gas	0.082	12:27
03 Room Air	0.000	12:28
04 Std. Gas	0.083	12:28
05 Room Air	0.000	12:29
06 Std. Gas	0.083	12:29
07 Room Air	0.000	12:29

Lot No = 14323080A4
Cyl No = 12
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check
needs cal adj.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 13:55

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:55
02 Std. Sol.	0.021	13:56
03 Room Air	0.000	13:56
04 Std. Sol.	0.019	13:57
05 Room Air	0.000	13:58
06 Std. Sol.	0.021	13:58
07 Room Air	0.000	13:59

08 Sim Temp = 34.0°C

Simul Ser No = MP3002

Std Sol No = 202301E

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: LOW AC - 0.020AC
Check

post cal adj.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 14:10

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:11
02 Std. Sol.	0.401	14:12
03 Room Air	0.000	14:12
04 Std. Sol.	0.403	14:13
05 Room Air	0.000	14:13
06 Std. Sol.	0.403	14:14
07 Room Air	0.000	14:15


08 Sim Temp = 34.0°C

Simul Ser No = MP6036

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC check - 0.400 AC
post cal adj.

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 14:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:19
02 Std. Gas	0.080	14:20
03 Room Air	0.000	14:20
04 Std. Gas	0.080	14:21
05 Room Air	0.000	14:21
06 Std. Gas	0.080	14:22
07 Room Air	0.000	14:22

Lot No = 14323080A4
Cyl No = 12
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

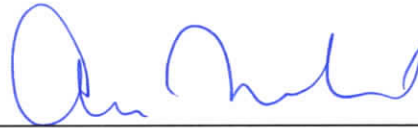

Operator Signature
ANNA NAREHOOD

Remarks: Dry Cal Check #1-3
post cal adj.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 14:24

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:24
02 Std. Gas	0.079	14:25
03 Room Air	0.000	14:25
04 Std. Gas	0.079	14:25
05 Room Air	0.000	14:26
06 Std. Gas	0.080	14:26
07 Room Air	0.000	14:27

Lot No = 14323080A4
Cyl No = 12
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6
post cal adj.

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004936
Location = TOXL 8164.14.00 09/16
04/29/2024 14:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:28
02 Std. Gas	0.079	14:28
03 Room Air	0.000	14:29
04 Std. Gas	0.079	14:29
05 Room Air	0.000	14:29
06 Std. Gas	0.080	14:30
07 Room Air	0.000	14:30

Lot No = 14323080A4
Cyl No = 12
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9
post cal adj.

Form 106-I8000