



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6509 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 01923080A3 Cyl. # 58)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: GFAP
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 905 psi Regulator: 1000 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3002
Lot #: 202301E
Exp. Date: 17Jan25
 Results ± 0.005 of known AC

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP10036
 Lot #: 202212C
 Exp. Date: 08Dec24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 14323080A4
 Cylinder #: 43
 Exp. Date: 4/5/25
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7344
 Lot #: ICS 8
 Exp. Date: N/A
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)



Test 1 <u>0.081</u>	Test 4 <u>0.081</u>	Test 7 <u>0.081</u>
Test 2 <u>0.080</u>	Test 5 <u>0.080</u>	Test 8 <u>0.081</u>
Test 3 <u>0.080</u>	Test 6 <u>0.080</u>	Test 9 <u>0.080</u>
Average <u>0.080</u>		

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No
 If No, state reason(s) why: _____

If Yes, change location code back to A.4.

<u></u>	<u>18 Apr 2024</u>
Inspector Signature	Date
<u></u>	<u>18 Apr 2024</u>
Reviewer	Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:20

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ & * () _ + ?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ & * () _ + ?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer (Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01923080A3
Standard Cyl #? 58
Standard Expiration? 02/05/2025
Oper No? 133237

Flow Cal. Date: 06/11/2019
Slope 445
Intercept 431160

IR Calibration Date: 06/11/2019
 3um 9um

0th Coef (*100): -27266 -14145
1st Coef (*100): 276865 139368
2nd Coef (*100): 2326 1158
H2O adj (mg/l*10k): 584 288

***** Printer Test End *****



Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:32

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:32
02 Std. Sol.	0.021	10:33
03 Room Air	0.000	10:34
04 Std. Sol.	0.022	10:34
05 Room Air	0.000	10:35
06 Std. Sol.	0.021	10:35
07 Room Air	0.000	10:36


08 Sim Temp = 34.0°C

Simul Ser No = MP3002

Std Sol No = 202301E

County = 08

Oper No. = 133237

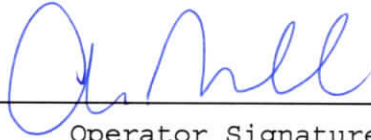

Operator Signature
ANNA NAREHOOD

Remarks: LOW AC CHECK - 0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:37

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:37
02 Std. Sol.	0.393	10:38
03 Room Air	0.000	10:39
04 Std. Sol.	0.394	10:40
05 Room Air	0.000	10:40
06 Std. Sol.	0.396	10:41
07 Room Air	0.000	10:41

08 Sim Temp = 34.0°C

Simul Ser No = MP6036
Std Sol No = 202212C
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC Check - 0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:44

Test	AC	Time
01 Room Air	0.000	10:45
02 *Subject Test	INT*	10:45
03 Room Air	0.000	10:46

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 43
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:46

Test	AC	Time
01 Diagnostic	OK	10:47
02 Room Air	RFI*	10:47
03 Room Air	0.000	10:48

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 43
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:48
02 Std. Gas	0.081	10:49
03 Room Air	0.000	10:49
04 Std. Gas	0.080	10:50
05 Room Air	0.000	10:50
06 Std. Gas	0.080	10:51
07 Room Air	0.000	10:51

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:52

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:52
02 Std. Gas	0.081	10:52
03 Room Air	0.000	10:53
04 Std. Gas	0.080	10:53
05 Room Air	0.000	10:54
06 Std. Gas	0.080	10:54
07 Room Air	0.000	10:55

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #46

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006509
Location = TOXL 8164.14.00 09/16
04/18/2024 10:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:56
02 Std. Gas	0.081	10:57
03 Room Air	0.000	10:57
04 Std. Gas	0.081	10:58
05 Room Air	0.000	10:58
06 Std. Gas	0.080	10:59
07 Room Air	0.000	10:59

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

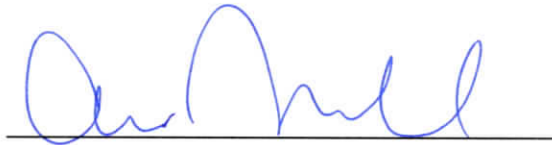

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000