



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6501 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
  - Gas Cylinder Yes or No (If Yes, Lot # 14323080A4 Cyl. # 5)
  - Keys Yes or No
  - Power Cord Yes or No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: MNAF
5.  Battery Check
  - Was the external battery pack replaced? Yes or No
6.  O-Rings
  - Replaced Simulator O-Ring Yes or No
  - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
  - Time Zone: CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).
  - Display: 991 psi Regulator: 1000 psi
  - Display and Regulator ± 50 psi of each other Yes or No
  - Gas tank tare necessary? Yes or No
  - If Yes, display readings after tare (Level 3,M,C,G):
  - Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

1.  Configure simulator for the following test (Level 1,S).
  - Wet Calibration Check - Low AC (Level 1,C)
  - Known Value ≤ 0.03 AC: 0.020 AC
  - Sim. Ser #: 202301E MP3002
  - Lot #: 202301E
  - Exp. Date: 1/Jan 25
  - Results ± 0.005 of known AC

- 2.  Configure simulator for the following test (Level 1,S).  
 Wet Calibration Check - High AC (Level 1,C)  
 Known Value  $\geq$  0.25 AC: 0.400 AC  
 Sim. Ser #: MP6036  
 Lot #: 202212C  
 Exp. Date: 08Dec24  
 Results  $\pm$  5% AC of known AC
- 3.  Configure dry gas standard for the remaining tests (Level 1,S).  
 Known Value : 0.080 AC  
 Gas Cylinder Lot #: 01923080A3  
 Cylinder #: 55  
 Exp. Date: 2/5/25
- 4.  Interferent Check (Level 1,B)  
 Known Value: 0.10 AC + 0.05% Acetone  
 Sim. Ser #: DR7344  
 Lot #: ICS 8  
 Exp. Date: N/A  
 Display reads "Interferent Detect"
- 5.  RFI Check (CMS Mode)  
 Display reads "RFI Detect"
- 6.  Dry Calibration Check (Level 1,C)  

Test 1	<u>0.081</u>	Test 4	<u>0.082</u>	Test 7	<u>0.082</u>
Test 2	<u>0.081</u>	Test 5	<u>0.081</u>	Test 8	<u>0.081</u>
Test 3	<u>0.081</u>	Test 6	<u>0.081</u>	Test 9	<u>0.082</u>
		Average	<u>0.081</u>		

 Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: N/A

---



---

Instrument is acceptable to be used in the field.  Yes or No  
 If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4.

[Signature]  
 Inspector Signature

19 Apr 2024  
 Date

[Signature]  
 Reviewer

25 Apr 2024  
 Date



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/19/2024      12:39

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:40
02 Std. Sol.	0.021	12:41
03 Room Air	0.000	12:41
04 Std. Sol.	0.021	12:42
05 Room Air	0.000	12:43
06 Std. Sol.	0.021	12:43
07 Room Air	0.000	12:44

08 Sim Temp = 34.0°C

Simul Ser No = MP3002  
Std Sol No = 202301E  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA NAREHOOD

Remarks: LOW AC CHECK - 0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/19/2024      12:45

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:46
02 Std. Sol.	0.392	12:46
03 Room Air	0.000	12:47
04 Std. Sol.	0.394	12:48
05 Room Air	0.000	12:48
06 Std. Sol.	0.395	12:49
07 Room Air	0.000	12:50


08 Sim Temp = 34.0°C

Simul Ser No = MP6036

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: High AC check - 0.400 AC

Form 106-I8000

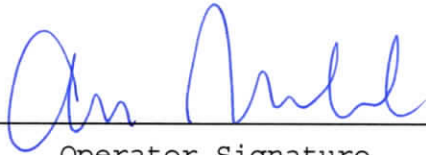
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/19/2024      12:51

Test	AC	Time
01 Room Air	0.000	12:52
02 *Subject Test	INT*	12:52
03 Room Air	0.000	12:53

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = INTERFERENT CK  
Dr. Lic. = ND/TES989643  
Lot No = 01923080A3  
Cyl No = 55  
Expiration Date = 02/05/2025  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/19/2024      12:54

Test	AC	Time
01 Diagnostic	OK	12:55
02 Room Air	RFI*	12:55
03 Room Air	0.000	12:55

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 01923080A3  
Cyl No = 55  
Expiration Date = 02/05/2025  
County = 08      Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/19/2024      12:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:56
02 Std. Gas	0.081	12:57
03 Room Air	0.000	12:57
04 Std. Gas	0.081	12:57
05 Room Air	0.000	12:58
06 Std. Gas	0.081	12:58
07 Room Air	0.000	12:59

Lot No = 01923080A3  
Cyl No = 55  
Exp Date = 02/05/2025  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: Dny cal check #1-3

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/19/2024      12:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:00
02 Std. Gas	0.082	13:00
03 Room Air	0.000	13:01
04 Std. Gas	0.081	13:01
05 Room Air	0.000	13:02
06 Std. Gas	0.081	13:02
07 Room Air	0.000	13:03

Lot No = 01923080A3  
Cyl No = 55  
Exp Date = 02/05/2025  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: *Dry cal check #44*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/19/2024      13:03

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:04
02 Std. Gas	0.082	13:04
03 Room Air	0.000	13:05
04 Std. Gas	0.081	13:05
05 Room Air	0.000	13:06
06 Std. Gas	0.082	13:06
07 Room Air	0.000	13:06

Lot No = 01923080A3  
Cyl No = 55  
Exp Date = 02/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry Cal check #7-9

Form 106-I8000