



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4196 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 14323080A4 Cyl. # 003)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: HETT
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 987 psi Regulator: 1000 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3002
Lot #: 202301E
Exp. Date: 17Jan25
 Results ± 0.005 of known AC

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP6036
 Lot #: 202212C
 Exp. Date: 08Dec24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 01923080A3
 Cylinder #: 18
 Exp. Date: 215125
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7344
 Lot #: ICS 8
 Exp. Date: NIA
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)

Test 1	<u>0.081</u>	Test 4	<u>0.081</u>	Test 7	<u>0.081</u>
Test 2	<u>0.080</u>	Test 5	<u>0.081</u>	Test 8	<u>0.080</u>
Test 3	<u>0.081</u>	Test 6	<u>0.080</u>	Test 9	<u>0.080</u>
Average				<u>0.080</u>	

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No
 If No, state reason(s) why: _____

If Yes, change location code back to A.4.

[Signature]
 Inspector Signature

05 June 2024
 Date

[Signature]
 Reviewer

05 June 2024
 Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
06/05/2024 11:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:35
02 Std. Sol.	0.019	11:36
03 Room Air	0.000	11:36
04 Std. Sol.	0.018	11:37
05 Room Air	0.000	11:38
06 Std. Sol.	0.018	11:38
07 Room Air	0.000	11:39


08 Sim Temp = 34.0°C

Simul Ser No = MP3002

Std Sol No = 202301E

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Low AC Check- 0.020Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
06/05/2024 11:40

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:40
02 Std. Sol.	0.384	11:41
03 Room Air	0.000	11:42
04 Std. Sol.	0.384	11:42
05 Room Air	0.000	11:43
06 Std. Sol.	0.384	11:44
07 Room Air	0.000	11:44

08 Sim Temp = 34.0°C

Simul Ser No = MP6036
Std Sol No = 202212C
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC check - 0.400AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
06/05/2024 11:50

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:51
02 Std. Gas	0.081	11:51
03 Room Air	0.000	11:52
04 Std. Gas	0.080	11:52
05 Room Air	0.000	11:52
06 Std. Gas	0.081	11:53
07 Room Air	0.000	11:53

Lot No = 01923080A3
Cyl No = 18
Exp Date = 02/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
06/05/2024 11:54

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:54
02 Std. Gas	0.081	11:55
03 Room Air	0.000	11:55
04 Std. Gas	0.081	11:55
05 Room Air	0.000	11:56
06 Std. Gas	0.080	11:56
07 Room Air	0.000	11:57

Lot No = 01923080A3
Cyl No = 18
Exp Date = 02/05/2025
County = 08 Oper No. = 133237

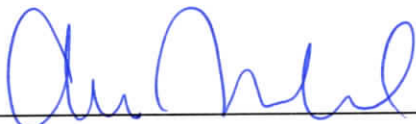

Operator Signature
ANNA NAREHOOD

Remarks: *dry cal check #4-6*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = TOXL 8164.14.00 09/16
06/05/2024 11:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:58
02 Std. Gas	0.081	11:58
03 Room Air	0.000	11:59
04 Std. Gas	0.080	11:59
05 Room Air	0.000	12:00
06 Std. Gas	0.080	12:00
07 Room Air	0.000	12:00

Lot No = 01923080A3
Cyl No = 18
Exp Date = 02/05/2025
County = 08 Oper No. = 133237


Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000