



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 0505 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # 14323080A1 Cyl. # 23)
Keys Yes or No
Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: MOHL
5. Battery Check
Was the external battery pack replaced? Yes or No
6. O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 945 psi Regulator: 1000 psi
Display and Regulator \pm 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: 950 psi Regulator: 1000 psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value \leq 0.03 AC: 0.020 AC
Sim. Ser #: MP3002
Lot #: 202301E
Exp. Date: 7Jan25
 Results \pm 0.005 of known AC

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP6036
 Lot #: 202212C
 Exp. Date: 08Dec24
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 01923080A3
 Cylinder #: 19
 Exp. Date: 215125
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7344
 Lot #: 1CS 8
 Exp. Date: NIA
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)

Test 1	<u>0.081</u>	Test 4	<u>0.081</u>	Test 7	<u>0.081</u>
Test 2	<u>0.080</u>	Test 5	<u>0.081</u>	Test 8	<u>0.082</u>
Test 3	<u>0.081</u>	Test 6	<u>0.081</u>	Test 9	<u>0.081</u>
		Average		<u>0.081</u>	

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No
 If No, state reason(s) why: _____

If Yes, change location code back to A.4.

[Signature]
 Inspector Signature

10 June 2024
 Date

[Signature]
 Reviewer

12 June 2024
 Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 11:50

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 14323080A1
Standard Cyl #? 23
Standard Expiration? 06/05/2025
Oper No? 133237

Flow Cal. Date: 08/20/2015
Slope 671
Intercept -642269

IR Calibration Date: 08/20/2015
 3um 9um

0th Coef(*100): -29025 -17051
1st Coef(*100): 252705 133345
2nd Coef(*100): 3840 1546
H2O adj(mg/l*10k): 817 461

***** Printer Test End *****

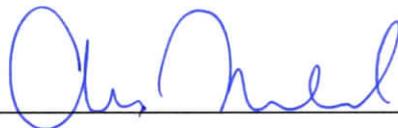

Operator Signature
ANNA NAREHOOD

Remarks: *Print Test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 11:51

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:51
02 Std. Sol.	0.021	11:52
03 Room Air	0.000	11:53
04 Std. Sol.	0.021	11:53
05 Room Air	0.000	11:54
06 Std. Sol.	0.020	11:55
07 Room Air	0.000	11:56

08 Sim Temp = 34.0°C

Simul Ser No = MP3002

Std Sol No = 202301E

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *LOW Ac check - 0.020Ac*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 11:57

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:57
02 Std. Sol.	0.398	11:59
03 Room Air	0.000	12:00
04 Std. Sol.	0.398	12:00
05 Room Air	0.000	12:01
06 Std. Sol.	0.399	12:02
07 Room Air	0.000	12:03

08 Sim Temp = 34.0°C

Simul Ser No = MP6036

Std Sol No = 202212C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High Ac Check - 0.400 Ac

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 12:06

Test	AC	Time
01 Room Air	0.000	12:07
02 *Subject Test	INT*	12:08
03 Room Air	0.000	12:08

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 01923080A3
Cyl No = 18
Expiration Date = 02/05/2025
County = 08 Oper No. = 133237

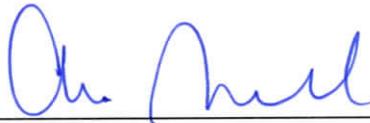

Operator Signature
ANNA NAREHOOD

Remarks: *interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 12:09

Test	AC	Time
01 Diagnostic	OK	12:10
02 Room Air	0.000	12:10
03 Reference	RFI*	12:11
04 Room Air	0.000	12:11

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK0
Dr. Lic. = ND/TES989643
Lot No = 01923080A3
Cyl No = 18
Expiration Date = 02/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

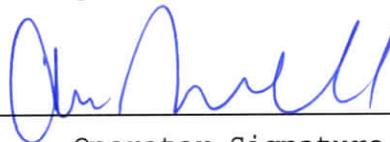

Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 12:11

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:12
02 Std. Gas	0.081	12:12
03 Room Air	0.000	12:13
04 Std. Gas	0.080	12:13
05 Room Air	0.000	12:14
06 Std. Gas	0.081	12:14
07 Room Air	0.000	12:15

Lot No = 01923080A3
Cyl No = 18
Exp Date = 02/05/2025
County = 08 Oper No. = 133237

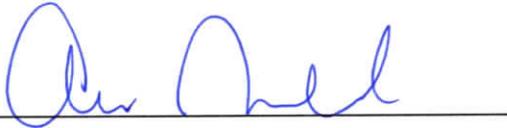

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 12:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:16
02 Std. Gas	0.081	12:16
03 Room Air	0.000	12:17
04 Std. Gas	0.081	12:17
05 Room Air	0.000	12:18
06 Std. Gas	0.081	12:18
07 Room Air	0.000	12:19

Lot No = 01923080A3
Cyl No = 18
Exp Date = 02/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Dry cal check # 4-6*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006505
Location = TOXL 8164.14.00 09/16
06/10/2024 12:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:20
02 Std. Gas	0.081	12:20
03 Room Air	0.000	12:21
04 Std. Gas	0.082	12:21
05 Room Air	0.000	12:22
06 Std. Gas	0.081	12:22
07 Room Air	0.000	12:23

Lot No = 01923080A3
Cyl No = 18
Exp Date = 02/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000