



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4191 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 01923080A3 Cyl. # 20)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: DUNN
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 967 psi Regulator: 1000 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3002
Lot #: 202301E
Exp. Date: 17Jan25
 Results ± 0.005 of known AC

- 2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.400 AC
 Sim. Ser #: MP6036
 Lot #: 202212C
 Exp. Date: 08DEC24
 Results \pm 5% AC of known AC
- 3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 14323080A4
 Cylinder #: 43
 Exp. Date: 615125
- 4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7344
 Lot #: 1CS 8
 Exp. Date: NIA
 Display reads "Interferent Detect"
- 5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
- 6. Dry Calibration Check (Level 1,C)

Test 1	<u>0.079</u>	Test 4	<u>0.080</u>	Test 7	<u>0.079</u>
Test 2	<u>0.080</u>	Test 5	<u>0.080</u>	Test 8	<u>0.080</u>
Test 3	<u>0.080</u>	Test 6	<u>0.080</u>	Test 9	<u>0.079</u>
		Average	<u>0.079</u>		

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4. NIA Instrument swapped

[Signature]
 Inspector Signature

25 June 2024
 Date

[Signature]
 Reviewer

25 June 2024
 Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 06:28

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01923080A3
Standard Cyl #? 20
Standard Expiration? 02/05/2025
Oper No? 133237

Flow Cal. Date: 01/28/2010
Slope 738
Intercept -777574

IR Calibration Date: 04/20/2017

	3um	9um
0th Coef(*100):	-8758	-19235
1st Coef(*100):	262182	129903
2nd Coef(*100):	3907	1462
H2O adj(mg/l*10k):	423	588

***** Printer Test End *****



Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 06:38

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	06:39
02 Std. Sol.	0.021	06:39
03 Room Air	0.000	06:40
04 Std. Sol.	0.021	06:41
05 Room Air	0.000	06:41
06 Std. Sol.	0.021	06:42
07 Room Air	0.000	06:42

08 Sim Temp = 34.0°C

Simul Ser No = MP3002
Std Sol No = 202301E
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: ~~Ø~~ Low AC check - 0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 07:00

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	07:00
02 Std. Sol.	0.392	07:01
03 Room Air	0.000	07:02
04 Std. Sol.	0.394	07:03
05 Room Air	0.000	07:03
06 Std. Sol.	0.394	07:04
07 Room Air	0.000	07:04

08 Sim Temp = 34.0°C

Simul Ser No = MP6036
Std Sol No = 202212C
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC check - 0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 07:08

Test	AC	Time
01 Room Air	0.000	07:09
02 *Subject Test	INT*	07:10
03 Room Air	0.000	07:10

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 43
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

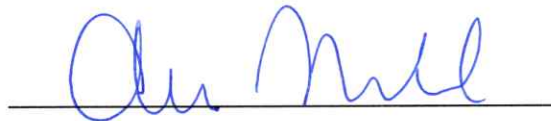

Operator Signature
ANNA NAREHOOD

Remarks: *interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 07:12

Test	AC	Time
01 Diagnostic	OK	07:13
02 Room Air	RFI*	07:13
03 Room Air	0.000	07:14

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 43
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 09:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:49
02 Std. Gas	0.079	09:49
03 Room Air	0.000	09:50
04 Std. Gas	0.080	09:50
05 Room Air	0.000	09:51
06 Std. Gas	0.080	09:51
07 Room Air	0.000	09:52

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 09:53

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:53
02 Std. Gas	0.080	09:54
03 Room Air	0.000	09:54
04 Std. Gas	0.080	09:55
05 Room Air	0.000	09:55
06 Std. Gas	0.080	09:55
07 Room Air	0.000	09:56

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

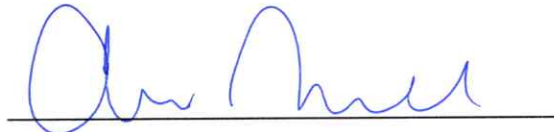

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004191
Location = TOXL 8164.14.00 09/16
06/25/2024 09:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:57
02 Std. Gas	0.079	09:58
03 Room Air	0.000	09:58
04 Std. Gas	0.080	09:58
05 Room Air	0.000	09:59
06 Std. Gas	0.079	09:59
07 Room Air	0.000	10:00

Lot No = 14323080A4
Cyl No = 43
Exp Date = 06/05/2025
County = 08 Oper No. = 133237


Operator Signature
ANNA NAREHOOD

Remarks: *Dry cal check #7-9*

Form 106-I8000