



ETHANOL GAS STANDARD CYLINDER REPORT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59282 (08/2018)

Chemical Test Operator Name (Print) <i>Cole, Adam W.</i>		
Location <i>6FPD</i>	Intoxilyzer® Serial Number <i>80-006678</i>	
Gas Lot Number <i>01524080A4</i>	Gas Cylinder Number <i>36</i>	Gas Expiration Date <i>03-05-2006</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
 Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. *0.084* AC
 - B. *0.082* AC
 - C. *0.083* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>Adam W. Cole</i> #642	Date <i>02-04-25</i>
Reviewed By (Crime Laboratory Use Only) Anna Narehood <i>Anna Narehood</i>	Date 11Feb2025


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006678
Location = GFPD 8164.14.00 09/16
02/04/2025 22:26

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	22:26
02 Std. Gas	0.084	22:27
03 Room Air	0.000	22:27
04 Std. Gas	0.082	22:28
05 Room Air	0.000	22:28
06 Std. Gas	0.083	22:28
07 Room Air	0.000	22:29

Lot No = 01524080A4
Cyl No = 36
Exp Date = 03/05/2026
County = 18 Oper No. = 133510

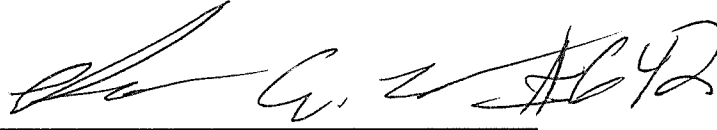

Operator Signature
ADAM COLE

Remarks:

Form 106-I8000