



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
 SFN 59281 (06/2018)

Serial Number <b>00-003006</b>	Instrument Location <b>1201 12th St SE, Ste C. Watford City, ND 58254</b>
Reason for Install/Repair	
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): N/A
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <b>[Signature]</b>	Date <b>2/5/25</b>
--	--------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <b>Anna Narehood</b>	<b>[Signature]</b>	Certified Date <b>05Feb2025</b>
--	--------------------	---------------------------------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-003066  
Location = MCSO 8164.14.00 09/16  
02/05/2025 08:37

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%\$%^&\*() +?

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%\$%^&\*() \_+?

Current Instrument Setup

Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Memfull? Yes  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.080  
Standard Lot #? 01524080A4  
Standard Cyl #? 17  
Standard Expiration? 03/05/2026  
Oper No? 132007  
  
Flow Cal. Date: 07/29/2010  
Slope 806  
Intercept -895033

IR Calibration Date: 07/29/2010  
3um 9um

-----  
0th Coef(\*100): -14075 -5808  
1st Coef(\*100): 272113 138204  
2nd Coef(\*100): 1637 986  
H2O adj(mg/l\*10k): 289 148

\*\*\*\*\* Printer Test End \*\*\*\*\*

*Kari Stuart*

Operator Signature  
KARI STUART

STATE OF NORTH DAKOTA }  
COUNTY OF MCKENZIE } ss

Remarks:

*APA-Print  
Fast*

I certify that the foregoing is a true and correct  
copy of the original document on file in this office.  
Dated at Watford City, North Dakota.

on this 5th day of FEBRUARY, 2025

*Kari Stuart*  
\_\_\_\_\_  
Watford City Sheriff's Department

Form 106-I8000

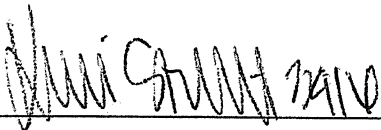
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003066  
Location = MCSO      8164.14.00 09/16  
02/05/2025      08:41

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:41
02 Std. Gas	0.081	08:42
03 Room Air	0.000	08:42
04 Std. Gas	0.079	08:42
05 Room Air	0.000	08:43
06 Std. Gas	0.081	08:43
07 Room Air	0.000	08:44

Lot No = 01524080A4  
Cyl No = 17  
Exp Date = 03/05/2026  
County = 27      Oper No. = 132007



Operator Signature  
KARI STUART

Remarks:


Cal check

Form 106-I8000

STATE OF NORTH DAKOTA } ss  
COUNTY OF MCKENZIE

I certify that the foregoing is a true and correct  
copy of the original document on file in this office.  
Dated at Watford City, North Dakota.

on this 07th day of February 2025

  
McKenzie County Sheriff's Department

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

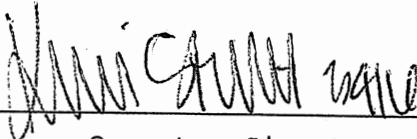
CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-003066  
Location = MCSO 8164.14.00 09/16  
02/05/2025 08:44

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	08:45
02 Room Air	RFI*	08:45

\*Invalid Test  
Inhibited - RFI

Lot No = 01524080A4  
Cyl No = 17  
Exp Date = 03/05/2026  
County = 27 Oper No. = 132007

  
Operator Signature  
KARI STUART

Remarks:

RFI TEST

Form 106-I8000

STATE OF NORTH DAKOTA  
COUNTY OF MCKENNA

I certify that the foregoing is a true and correct copy of the original document on file in this office.  
Dated at Watford City, North Dakota.

on this 17th day of February, 2025  
