



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4189 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # 14323080A1 Cyl. # 72)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: NTPD
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 825 psi Regulator: 800 psi
Display and Regulator \pm 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value \leq 0.03 AC: 0.020 AC
Sim. Ser #: MP5321
Lot #: 202311D
Exp. Date: 11/28/25
☒ Results \pm 0.005 of known AC

Intoxilyzer 8000 Annual Inspection

Laboratory Unit: Toxicology Unit - Breath Alcohol Section

Approved By: Laboratory Director

UNCONTROLLED WHEN PRINTED

Document ID: 11698 Revision: 3

Status: Published

Date Approved: 03/20/2025

Page 1 of 2


2. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - High AC (Level 1,C)
Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP6035
Lot #: 202402C
Exp. Date: 2/14/26
☒ Results $\pm 5\%$ AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).
Known Value : 0.080 AC
Gas Cylinder Lot #: 14323080A4
Cylinder #: 618 den 4/23/25
Exp. Date: 6/5/25
4. ☒ Interferent Check (Level 1,B)
Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7352
Lot #: ICS 8
Exp. Date: None
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)
- | | | |
|----------------------|---------------------|---------------------|
| Test 1 <u>0.081</u> | Test 4 <u>0.081</u> | Test 7 <u>0.081</u> |
| Test 2 <u>0.080</u> | Test 5 <u>0.080</u> | Test 8 <u>0.080</u> |
| Test 3 <u>0.081</u> | Test 6 <u>0.081</u> | Test 9 <u>0.081</u> |
| Average <u>0.080</u> | | |
- ☒ Results ± 0.005 AC of known AC

D. Remarks/Maintenance: N/A


Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒


Inspector Signature

23 April 2025
Date


Reviewer

24 Apr 2025
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:13

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 14323080A1
Standard Cyl #? 72
Standard Expiration? 06/05/2025
Oper No? 133237

Flow Cal. Date: 02/02/2011
Slope 628
Intercept -452608

IR Calibration Date: 05/19/2016
 3um 9um

| | | |
|--------------------|--------|--------|
| 0th Coef(*100): | -17767 | -18761 |
| 1st Coef(*100): | 263439 | 133606 |
| 2nd Coef(*100): | 1960 | 1140 |
| H2O adj(mg/l*10k): | 341 | 362 |

***** Printer Test End *****



Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:18

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 12:18 |
| 02 Std. Sol. | 0.022 | 12:19 |
| 03 Room Air | 0.000 | 12:20 |
| 04 Std. Sol. | 0.022 | 12:21 |
| 05 Room Air | 0.000 | 12:21 |
| 06 Std. Sol. | 0.022 | 12:22 |
| 07 Room Air | 0.000 | 12:22 |

08 Sim Temp = 34.0°C

Simul Ser No = MP5321
Std Sol No = 202311D
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Low AC Check - 0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:28

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 12:28 |
| 02 Std. Sol. | 0.298 | 12:29 |
| 03 Room Air | 0.000 | 12:30 |
| 04 Std. Sol. | 0.299 | 12:30 |
| 05 Room Air | 0.000 | 12:31 |
| 06 Std. Sol. | 0.299 | 12:32 |
| 07 Room Air | 0.000 | 12:32 |

08 Sim Temp = 34.0°C

Simul Ser No = MP6035
Std Sol No = 202402C
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC check - 0.300AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:33

| Test | AC | Time |
|------------------|-------|-------|
| 01 Room Air | 0.000 | 12:34 |
| 02 *Subject Test | INT* | 12:35 |
| 03 Room Air | 0.000 | 12:36 |

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 18
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Interferent check*
0.10AL + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:36

| Test | AC | Time |
|---------------|-------|-------|
| 01 Diagnostic | OK | 12:37 |
| 02 Room Air | RFI* | 12:37 |
| 03 Room Air | 0.000 | 12:37 |

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 18
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:38

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 12:38 |
| 02 Std. Gas | 0.081 | 12:38 |
| 03 Room Air | 0.000 | 12:39 |
| 04 Std. Gas | 0.080 | 12:39 |
| 05 Room Air | 0.000 | 12:40 |
| 06 Std. Gas | 0.081 | 12:40 |
| 07 Room Air | 0.000 | 12:41 |

Lot No = 14323080A4
Cyl No = 18
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

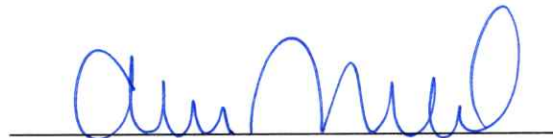

Operator Signature
ANNA NAREHOOD

Remarks: DRYCAL check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:41

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 12:42 |
| 02 Std. Gas | 0.081 | 12:42 |
| 03 Room Air | 0.000 | 12:42 |
| 04 Std. Gas | 0.080 | 12:43 |
| 05 Room Air | 0.000 | 12:43 |
| 06 Std. Gas | 0.081 | 12:44 |
| 07 Room Air | 0.000 | 12:44 |

Lot No = 14323080A4
Cyl No = 18
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = TOXL 8164.14.00 09/16
04/23/2025 12:44

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 12:45 |
| 02 Std. Gas | 0.081 | 12:45 |
| 03 Room Air | 0.000 | 12:46 |
| 04 Std. Gas | 0.080 | 12:46 |
| 05 Room Air | 0.000 | 12:47 |
| 06 Std. Gas | 0.081 | 12:47 |
| 07 Room Air | 0.000 | 12:48 |

Lot No = 14323080A4
Cyl No = 18
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000