



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6682 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # 25024080A3 Cyl. # 1)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: CRDS
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 961 psi Regulator: 1000 psi
Display and Regulator $\pm$ 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value $\leq$ 0.03 AC: 0.020 AC
Sim. Ser #: MP5321
Lot #: 202311D
Exp. Date: 11/28/25
☒ Results $\pm$ 0.005 of known AC

2. ☒ Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value ≥ 0.25 AC: 0.300 AC
 Sim. Ser #: MP6035
 Lot #: 202402C
 Exp. Date: 2/14/26
☒ Results $\pm 5\%$ AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 14323080A1
 Cylinder #: 72
 Exp. Date: 01/5/25
4. ☒ Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7352
 Lot #: ICS8
 Exp. Date: None
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)

Test 1 <u>0.080</u>	Test 4 <u>0.081</u>	Test 7 <u>0.081</u>
Test 2 <u>0.080</u>	Test 5 <u>0.080</u>	Test 8 <u>0.080</u>
Test 3 <u>0.081</u>	Test 6 <u>0.080</u>	Test 9 <u>0.080</u>
Average <u>0.080</u>		

☒ Results ± 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

Inspector Signature

Date

Reviewer

Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = TOXL 8164.14.00 09/16
04/28/2025 14:48


WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:48
02 Std. Sol.	0.019	14:49
03 Room Air	0.000	14:50
04 Std. Sol.	0.020	14:51
05 Room Air	0.000	14:51
06 Std. Sol.	0.020	14:52
07 Room Air	0.000	14:52

08 Sim Temp = 34.0°C

Simul Ser No = MP5321
Std Sol No = 202311D
County = 08

Oper No. = 133237

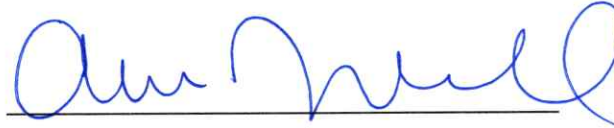

Operator Signature
ANNA NAREHOOD

Remarks: LOW AC check - 0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = TOXL 8164.14.00 09/16
04/28/2025 14:58

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:58
02 Std. Sol.	0.295	14:59
03 Room Air	0.000	15:00
04 Std. Sol.	0.296	15:00
05 Room Air	0.000	15:01
06 Std. Sol.	0.297	15:02
07 Room Air	0.000	15:02


08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC Check - 0.300AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = TOXL 8164.14.00 09/16
04/28/2025 15:03

Test	AC	Time
01 Room Air	0.000	15:04
02 *Subject Test	INT*	15:05
03 Room Air	0.000	15:05

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A1
Cyl No = 72
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent check
0.10Ac + 0.059% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = TOXL 8164.14.00 09/16
04/28/2025 15:06

Test	AC	Time
01 Diagnostic	OK	15:06
02 Room Air	0.000	15:07
03 *Subject Test	RFI*	15:07
04 Room Air	0.000	15:07

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A1
Cyl No = 72
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = TOXL 8164.14.00 09/16
04/28/2025 15:08

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:09
02 Std. Gas	0.080	15:09
03 Room Air	0.000	15:10
04 Std. Gas	0.080	15:10
05 Room Air	0.000	15:11
06 Std. Gas	0.081	15:11
07 Room Air	0.000	15:12

Lot No = 14323080A1
Cyl No = 72
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

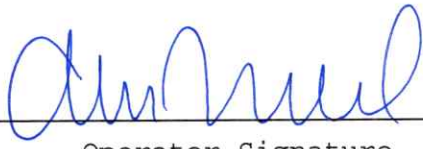

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = TOXL 8164.14.00 09/16
04/28/2025 15:12

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:13
02 Std. Gas	0.081	15:13
03 Room Air	0.000	15:13
04 Std. Gas	0.080	15:14
05 Room Air	0.000	15:14
06 Std. Gas	0.080	15:15
07 Room Air	0.000	15:15

Lot No = 14323080A1
Cyl No = 72
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

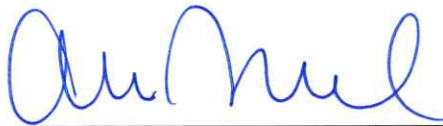

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check # 4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = TOXL 8164.14.00 09/16
04/28/2025 15:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:16
02 Std. Gas	0.081	15:16
03 Room Air	0.000	15:17
04 Std. Gas	0.080	15:17
05 Room Air	0.000	15:18
06 Std. Gas	0.080	15:18
07 Room Air	0.000	15:19

Lot No = 14323080A1
Cyl No = 72
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

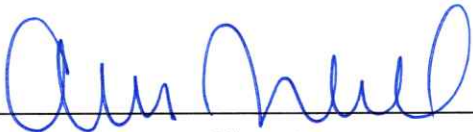

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000