



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6671

Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # 25024080A3 Cyl. # 4)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: DEVL
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 834 psi Regulator: 850 psi
Display and Regulator $\pm$ 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value $\leq$ 0.03 AC: 0.020 AC
Sim. Ser #: MP5321
Lot #: 202311D
Exp. Date: 11/28/25
☒ Results $\pm$ 0.005 of known AC

2. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - High AC (Level 1,C)
Known Value $\geq$ 0.25 AC: 0.300 AC
Sim. Ser #: MP6035
Lot #: 202402C
Exp. Date: 2/14/26
☒ Results $\pm$ 5% AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).
Known Value : 0.080 AC
Gas Cylinder Lot #: 14323080A1
Cylinder #: 71
Exp. Date: 6/5/25
4. ☒ Interferent Check (Level 1,B)
Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7352
Lot #: ICS8
Exp. Date: None
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)
Test 1 0.081 Test 4 0.081 Test 7 0.081
Test 2 0.081 Test 5 0.081 Test 8 0.081
Test 3 0.081 Test 6 0.081 Test 9 0.081
Average 0.081
☒ Results $\pm$ 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

[Signature]
Inspector Signature

28 Apr 12025
Date

[Signature]
Reviewer

29 Apr. 2025
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 13:46

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 25024080A3
Standard Cyl #? 4
Standard Expiration? 10/05/2026
Oper No? 133237

Flow Cal. Date: 08/22/2016
Slope 703
Intercept -691868

IR Calibration Date: 08/22/2016
 3um 9um

0th Coef(*100): -17135 -24345
1st Coef(*100): 254798 132856
2nd Coef(*100): 3386 1354
H2O adj(mg/l*10k): 610 539

***** Printer Test End *****



Operator Signature
ANNA NAREHOOD

Remarks: print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 13:49

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:50
02 Std. Sol.	0.019	13:51
03 Room Air	0.000	13:51
04 Std. Sol.	0.020	13:52
05 Room Air	0.000	13:52
06 Std. Sol.	0.020	13:53
07 Room Air	0.000	13:54


08 Sim Temp = 34.0°C

Simul Ser No = MP5321

Std Sol No = 202311D

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: LOW AC CHECK - 0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 13:56

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:57
02 Std. Sol.	0.292	13:57
03 Room Air	0.000	13:58
04 Std. Sol.	0.294	13:59
05 Room Air	0.000	13:59
06 Std. Sol.	0.295	14:00
07 Room Air	0.000	14:01


08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC check - 0.300AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 14:05

Test	AC	Time
01 Room Air	0.000	14:06
02 *Subject Test	INT*	14:06
03 Room Air	0.000	14:07

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A1
Cyl No = 71
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Interferent Check*
0.10Ac + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 14:08

Test	AC	Time
01 Diagnostic	OK	14:08
02 Room Air	RFI*	14:09
03 Room Air	0.000	14:09

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A1
Cyl No = 71
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 14:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:10
02 Std. Gas	0.081	14:10
03 Room Air	0.000	14:11
04 Std. Gas	0.081	14:11
05 Room Air	0.000	14:12
06 Std. Gas	0.081	14:12
07 Room Air	0.000	14:13

Lot No = 14323080A1
Cyl No = 71
Exp Date = 06/05/2025
County = 08 Oper No. = 133237


Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check # 1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 14:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:14
02 Std. Gas	0.081	14:14
03 Room Air	0.000	14:14
04 Std. Gas	0.081	14:15
05 Room Air	0.000	14:15
06 Std. Gas	0.081	14:16
07 Room Air	0.000	14:16

Lot No = 14323080A1
Cyl No = 71
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

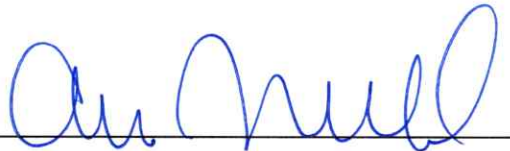

Operator Signature
ANNA NAREHOOD

Remarks: Dry Cal check #4-6

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006671
Location = TOXL 8164.14.00 09/16
04/28/2025 14:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:17
02 Std. Gas	0.081	14:17
03 Room Air	0.000	14:18
04 Std. Gas	0.081	14:18
05 Room Air	0.000	14:19
06 Std. Gas	0.081	14:19
07 Room Air	0.000	14:20

Lot No = 14323080A1
Cyl No = 71
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000