



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
SFN 59281 (06/2018)

Serial Number 80-006682	Instrument Location CRS
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- ☒ 1. Surge Protector Installed/Property Grounded.
- ☒ 2. Telephone Line Connected to Intoxilyzer® 8000.
- ☒ 3. Breath Tube Heated.
- ☒ 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- ☒ 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- ☒ 6. Run Tests:
 - ☒ A. Print Test (Level 1, Function P).
 - ☒ B. ACA Test (Level 1, Function C).
 - ☒ C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- ☒ 7. Repair and/or Maintenance Performed (If any): _____
- ☐ 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place It by the Intoxilyzer® for Use.
- ☒ 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- ☐ 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date 4-29-25
-------------------------------	------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By Anna Narehood	Certified Date 30 April 2025
---	--

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = CROS 8164.14.00 09/16
04/29/2025 22:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	22:42
02 Std. Gas	0.082	22:43
03 Room Air	0.000	22:43
04 Std. Gas	0.081	22:44
05 Room Air	0.000	22:44
06 Std. Gas	0.081	22:45
07 Room Air	0.000	22:45


Lot No = 232492

Cyl No = 1

Exp Date = 10/05/2026

County = 12

Oper No. = 134037

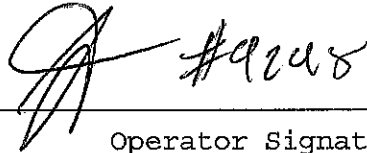

Operator Signature
JAMES STACEY

Remarks:

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006682
Location = CROS 8164.14.00 09/16
04/29/2025 22:46

Test	AC	Time
01 Room Air	0.000	22:48
02 *Subject Test	RFI*	22:49
03 Room Air	0.000	22:49

*Invalid Test
Inhibited - RFI

Sub Name = DUMMY, DUMMY L
Sub DOB = 09/09/2000
Sub Sex = Male Weight = 230
Test = OTH Cit = 1
Dr. Lic. = ND/NA
Lot No = 232492
Cyl No = 1
Expiration Date = 10/05/2026
County = 12 Oper No. = 134037

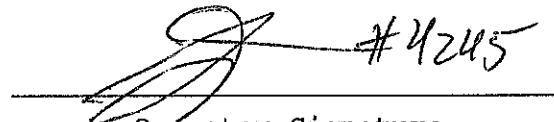
Operator Signature
JAMES STACEY

Remarks:

RFI

Form 106-I8000