



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 5946 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # 14323080A1 Cyl. # 22)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: FINL
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 940 psi Regulator: 950 psi
Display and Regulator \pm 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value \leq 0.03 AC: 0.020 AC
Sim. Ser #: MP5321
Lot #: 202311D
Exp. Date: 11/28/25
☒ Results \pm 0.005 of known AC

2. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - High AC (Level 1,C)
Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: 202402C MP6035 allw 518125
Lot #: 2114126 202402C
Exp. Date: 2/14/26
☒ Results $\pm 5\%$ AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).
Known Value : 0.080 AC
Gas Cylinder Lot #: 14323080A4
Cylinder #: 42
Exp. Date: 6/5/25
4. ☒ Interferent Check (Level 1,B)
Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7352
Lot #: 1CS8
Exp. Date: None
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)
Test 1 0.080 Test 4 0.081 Test 7 0.080
Test 2 0.081 Test 5 0.081 Test 8 0.082
Test 3 0.081 Test 6 0.082 Test 9 0.082
Average 0.081
☒ Results ± 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

[Signature]
Inspector Signature

08 May 2025
Date

[Signature]
Reviewer

08 May 2025
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 09:51

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?


Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 14323080A1
Standard Cyl #? 22
Standard Expiration? 06/05/2025
Oper No? 133237

Flow Cal. Date: 06/02/2021
Slope 642
Intercept -600927

IR Calibration Date:	06/02/2021
	3um 9um
0th Coef(*100):	-20165 -16483
1st Coef(*100):	290371 141330
2nd Coef(*100):	953 910
H2O adj(mg/l*10k):	496 404

***** Printer Test End *****

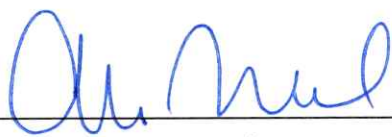

Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 10:29

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:30
02 Std. Sol.	0.022	10:31
03 Room Air	0.000	10:31
04 Std. Sol.	0.022	10:32
05 Room Air	0.000	10:32
06 Std. Sol.	0.022	10:33
07 Room Air	0.000	10:34

08 Sim Temp = 34.0°C

Simul Ser No = MP5321
Std Sol No = 202311D
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: LOW Ac check - 0.020Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 10:35

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:35
02 Std. Sol.	0.296	10:36
03 Room Air	0.000	10:37
04 Std. Sol.	0.297	10:37
05 Room Air	0.000	10:38
06 Std. Sol.	0.297	10:39
07 Room Air	0.000	10:39


08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237

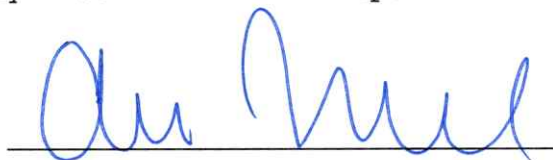

Operator Signature
ANNA NAREHOOD

Remarks: High AC Check - 0.300AE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 10:40

Test	AC	Time
01 Room Air	0.000	10:41
02 *Subject Test	INT*	10:41
03 Room Air	0.000	10:42

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 42
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent check
0.10AC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 10:43

Test	AC	Time
01 Diagnostic	OK	10:43
02 Room Air	0.000	10:44
03 *Subject Test	RFI*	10:44
04 Room Air	0.000	10:45

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 42
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI Check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 10:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:49
02 Std. Gas	0.080	10:49
03 Room Air	0.000	10:50
04 Std. Gas	0.081	10:50
05 Room Air	0.000	10:51
06 Std. Gas	0.081	10:51
07 Room Air	0.000	10:52

Lot No = 14323080A4
Cyl No = 42
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: DRY cal check #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 10:52

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:53
02 Std. Gas	0.081	10:53
03 Room Air	0.000	10:54
04 Std. Gas	0.081	10:54
05 Room Air	0.000	10:55
06 Std. Gas	0.082	10:55
07 Room Air	0.000	10:56

Lot No = 14323080A4
Cyl No = 42
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

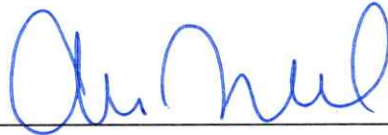

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005946
Location = TOXL 8164.14.00 09/16
05/08/2025 10:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:57
02 Std. Gas	0.080	10:57
03 Room Air	0.000	10:57
04 Std. Gas	0.082	10:58
05 Room Air	0.000	10:58
06 Std. Gas	0.082	10:59
07 Room Air	0.000	10:59

Lot No = 14323080A4
Cyl No = 42
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

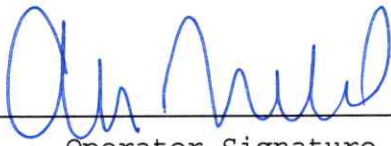

Operator Signature
ANNA NAREHOOD

Remarks: Dry Cal Check #7-9

Form 106-I8000