



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6491 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # M323080A1 Cyl. # 19)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: WESO
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 726 psi Regulator: 750 psi
Display and Regulator $\pm$ 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value $\leq$ 0.03 AC: 0.020 AC
Sim. Ser #: MP5321
Lot #: 202311D
Exp. Date: 11/28/25
☒ Results $\pm$ 0.005 of known AC

2. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - High AC (Level 1,C)
Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP6035
Lot #: 202402C
Exp. Date: 2/14/26
☒ Results $\pm 5\%$ AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).
Known Value : 0.080 AC
Gas Cylinder Lot #: 1432308DAY
Cylinder #: 14
Exp. Date: 015125
4. ☒ Interferent Check (Level 1,B)
Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7352
Lot #: ICS8
Exp. Date: None
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)
Test 1 0.081 Test 4 0.081 Test 7 0.082
Test 2 0.082 Test 5 0.082 Test 8 0.082
Test 3 0.081 Test 6 0.081 Test 9 0.081
Average 0.081
☒ Results ± 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

[Signature]
Inspector Signature

20 May 2025
Date

[Signature]
Reviewer

21 May 2025
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:08

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Wet
Standard Value? 0.020
Standard Solution #? 202311D
Sim Serial #? MP5321
Oper No? 133237

Flow Cal. Date: 05/22/2018
Slope 639
Intercept -618311

IR Calibration Date: 05/23/2018
3um 9um

0th Coef(*100):	-23641	-17066
1st Coef(*100):	264855	137703
2nd Coef(*100):	2663	1471
H2O adj(mg/l*10k):	556	451

***** Printer Test End *****

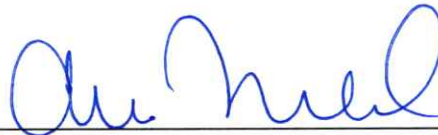

Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:08

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:09
02 Std. Sol.	0.020	11:10
03 Room Air	0.000	11:10
04 Std. Sol.	0.020	11:11
05 Room Air	0.000	11:12
06 Std. Sol.	0.021	11:12
07 Room Air	0.000	11:13

08 Sim Temp = 34.0°C

Simul Ser No = MP5321
Std Sol No = 202311D
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: LOW AC CHECK - 0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:15

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:15
02 Std. Sol.	0.296	11:16
03 Room Air	0.000	11:17
04 Std. Sol.	0.294	11:18
05 Room Air	0.000	11:18
06 Std. Sol.	0.295	11:19
07 Room Air	0.000	11:20

08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High Ac Check - 0.300Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:21

Test	AC	Time
01 Room Air	0.000	11:22
02 *Subject Test	INT*	11:22
03 Room Air	0.000	11:23

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 14
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent check
0.10Ac + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:25

Test	AC	Time
01 Diagnostic	OK	11:26
02 Room Air	0.000	11:26
03 *Subject Test	RFI*	11:26
04 Room Air	0.000	11:27

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 14323080A4
Cyl No = 14
Expiration Date = 06/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:29
02 Std. Gas	0.081	11:29
03 Room Air	0.000	11:30
04 Std. Gas	0.082	11:30
05 Room Air	0.000	11:31
06 Std. Gas	0.081	11:31
07 Room Air	0.000	11:32

Lot No = 14323080A4
Cyl No = 14
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:32

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:33
02 Std. Gas	0.081	11:33
03 Room Air	0.000	11:34
04 Std. Gas	0.082	11:34
05 Room Air	0.000	11:35
06 Std. Gas	0.081	11:35
07 Room Air	0.000	11:35

Lot No = 14323080A4
Cyl No = 14
Exp Date = 06/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006491
Location = TOXL 8164.14.00 09/16
05/20/2025 11:36

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:36
02 Std. Gas	0.082	11:37
03 Room Air	0.000	11:37
04 Std. Gas	0.082	11:37
05 Room Air	0.000	11:38
06 Std. Gas	0.081	11:38
07 Room Air	0.000	11:39

Lot No = 14323080A4
Cyl No = 14
Exp Date = 06/05/2025
County = 08 Oper No. = 133237

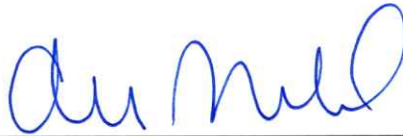

Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000