



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6690 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 14323080A4 Cyl. # 11)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: SACO
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 1000 psi Regulator: 1000 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP5321
Lot #: 2023110
Exp. Date: 11/28/25
 Results ± 0.005 of known AC

2. Configure simulator for the following test (Level 1,S).
 Wet Calibration Check - High AC (Level 1,C)
 Known Value \geq 0.25 AC: 0.300 AC
 Sim. Ser #: MP6035
 Lot #: 202402C
 Exp. Date: 2/14/26
 Results \pm 5% AC of known AC
3. Configure dry gas standard for the remaining tests (Level 1,S).
 Known Value : 0.080 AC
 Gas Cylinder Lot #: 28423080A3
 Cylinder #: 41
 Exp. Date: 11/5/25
4. Interferent Check (Level 1,B)
 Known Value: 0.10 AC + 0.05% Acetone
 Sim. Ser #: DR7352
 Lot #: ICS 8
 Exp. Date: None
 Display reads "Interferent Detect"
5. RFI Check (CMS Mode)
 Display reads "RFI Detect"
6. Dry Calibration Check (Level 1,C)

Test 1 <u>0.080</u>	Test 4 <u>0.082</u>	Test 7 <u>0.081</u>
Test 2 <u>0.081</u>	Test 5 <u>0.080</u>	Test 8 <u>0.081</u>
Test 3 <u>0.081</u>	Test 6 <u>0.080</u>	Test 9 <u>0.081</u>
Average <u>0.080</u>		

 Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No
 If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL.

<u><i>[Signature]</i></u>	<u>MAY 27, 2025</u>
Inspector Signature	Date
<u><i>[Signature]</i></u>	<u>28 May 2025</u>
Reviewer	Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 13:36

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer (Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 14323080A4
Standard Cyl #? 11
Standard Expiration? 06/05/2025
Oper No? 133237

Flow Cal. Date: 08/23/2018
Slope 677
Intercept -593298

IR Calibration Date: 08/23/2018

	3um	9um
0th Coef(*100):	-8380	-21663
1st Coef(*100):	265142	130429
2nd Coef(*100):	3933	1429
H2O adj(mg/l*10k):	412	539

***** Printer Test End *****



Operator Signature
ANNA NAREHOOD

Remarks: Print Test

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 13:45

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:46
02 Std. Sol.	0.019	13:46
03 Room Air	0.000	13:47
04 Std. Sol.	0.019	13:48
05 Room Air	0.000	13:48
06 Std. Sol.	0.019	13:49
07 Room Air	0.000	13:49

08 Sim Temp = 34.0°C

Simul Ser No = MP5321

Std Sol No = 202311D

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Low AC Check - 0.020 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 13:57

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:57
02 Std. Sol.	0.295	13:58
03 Room Air	0.000	13:59
04 Std. Sol.	0.295	13:59
05 Room Air	0.000	14:00
06 Std. Sol.	0.295	14:01
07 Room Air	0.000	14:01

08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC Check -0.300AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 14:02

Test	AC	Time
01 Room Air	0.000	14:03
02 *Subject Test	INT*	14:04
03 Room Air	0.000	14:04

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent check
0.10AC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 14:05

Test	AC	Time
01 Diagnostic	OK	14:05
02 Room Air	0.000	14:06
03 *Subject Test	RFI*	14:06
04 Room Air	0.000	14:07

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 14:07

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:08
02 Std. Gas	0.080	14:08
03 Room Air	0.000	14:09
04 Std. Gas	0.081	14:09
05 Room Air	0.000	14:10
06 Std. Gas	0.081	14:10
07 Room Air	0.000	14:11

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237

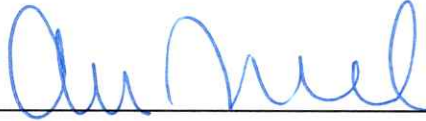

Operator Signature
ANNA NAREHOOD

Remarks: *Dry cal check #1-3*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 14:11

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:12
02 Std. Gas	0.082	14:12
03 Room Air	0.000	14:13
04 Std. Gas	0.080	14:13
05 Room Air	0.000	14:14
06 Std. Gas	0.080	14:14
07 Room Air	0.000	14:15

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Dry Cal check #4-6*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/27/2025 14:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:15
02 Std. Gas	0.081	14:16
03 Room Air	0.000	14:16
04 Std. Gas	0.081	14:17
05 Room Air	0.000	14:17
06 Std. Gas	0.081	14:18
07 Room Air	0.000	14:18

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237

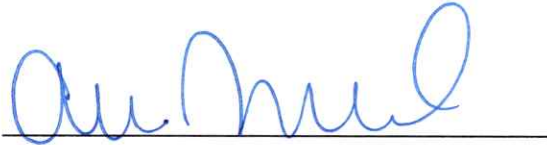

Operator Signature
ANNA NAREHOOD

Remarks: *Dry cal check #7-9*

Form 106-I8000