



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6501 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:  
Gas Cylinder Yes or No (If Yes, Lot # 14323080A4 Cyl. # 5)  
Keys Yes or No  
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: MNAF
5. ☒ Battery Check  
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings  
Replaced Simulator O-Ring Yes or No  
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).  
Display: 830 psi Regulator: 800 psi  
Display and Regulator  $\pm$  50 psi of each other Yes or No  
Gas tank tare necessary? Yes or No  
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value  $\leq$  0.03 AC: 0.020 AC  
Sim. Ser #: MP5321  
Lot #: 262311D  
Exp. Date: 11/28/25  
☒ Results  $\pm$  0.005 of known AC

2. ☒ Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - High AC (Level 1,C)  
Known Value  $\geq$  0.25 AC: 0.300 AC  
Sim. Ser #: MP6035  
Lot #: 202402C  
Exp. Date: 02/14/26  
☒ Results  $\pm$  5% AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).  
Known Value : 0.080 AC  
Gas Cylinder Lot #: 14323080A1  
Cylinder #: 64  
Exp. Date: 6/5/25
4. ☒ Interferent Check (Level 1,B)  
Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR7352  
Lot #: ICS8  
Exp. Date: None  
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)  
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)  
Test 1 0.081 Test 4 0.081 Test 7 0.081  
Test 2 0.080 Test 5 0.080 Test 8 0.081  
Test 3 0.080 Test 6 0.080 Test 9 0.080  
Average 0.080  
☒ Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

[Signature]  
Inspector Signature

04 Apr 2025  
Date

[Signature]  
Reviewer

07 Apr 2025  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:33

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&\*()\_+?

Current Instrument Setup


Data Entry Mode:      Enabled  
Start Test Sequence:      DABACABA  
Display Prelim Rslt?      Yes  
Display Third Digit?      Yes  
Inhib Printer(Y/N)?      No  
Display Volume?      No  
Disable On Memfull?      Yes  
# of Print Copies?      1  
Select Std (D/W/I)?      Dry  
Standard Value?      0.080  
Standard Lot #?      14323080A1  
Standard Cyl #?      69  
Standard Expiration?      06/05/2025  
Oper No?      133237

Flow Cal. Date:      06/13/2019  
Slope      651  
Intercept      -777821

IR Calibration Date:      06/13/2019  
   3um      9um

|                    |        |        |
|--------------------|--------|--------|
| 0th Coef(*100):    | -20531 | -14906 |
| 1st Coef(*100):    | 270252 | 139749 |
| 2nd Coef(*100):    | 1917   | 1284   |
| H2O adj(mg/l*10k): | 393    | 321    |

\*\*\*\*\* Printer Test End \*\*\*\*\*

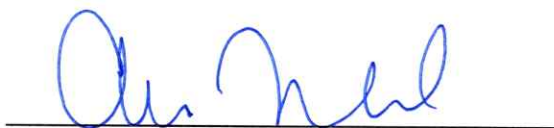

Operator Signature  
ANNA NAREHOOD

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:11

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 15:12 |
| 02 Std. Sol. | 0.021 | 15:13 |
| 03 Room Air  | 0.000 | 15:13 |
| 04 Std. Sol. | 0.022 | 15:14 |
| 05 Room Air  | 0.000 | 15:14 |
| 06 Std. Sol. | 0.022 | 15:15 |
| 07 Room Air  | 0.000 | 15:16 |


08 Sim Temp = 34.0°C

Simul Ser No = MP5321

Std Sol No = 202311D

County = 08

Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: LOW AC Check -0.020 AC

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:16

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 15:17 |
| 02 Std. Sol. | 0.298 | 15:18 |
| 03 Room Air  | 0.000 | 15:18 |
| 04 Std. Sol. | 0.305 | 15:19 |
| 05 Room Air  | 0.000 | 15:20 |
| 06 Std. Sol. | 0.306 | 15:21 |
| 07 Room Air  | 0.000 | 15:21 |


08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: High Ac Check - 0.300Ac

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:22

| Test             | AC    | Time  |
|------------------|-------|-------|
| 01 Room Air      | 0.000 | 15:23 |
| 02 *Subject Test | INT*  | 15:24 |
| 03 Room Air      | 0.000 | 15:25 |

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = INTERFERENT CK  
Dr. Lic. = ND/TES989643  
Lot No = 14323080A1  
Cyl No = 69  
Expiration Date = 06/05/2025  
County = 08      Oper No. = 133237

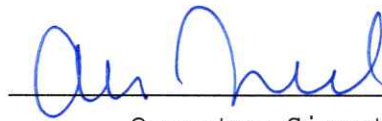  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: Interferent check  
0.10AC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:25

| Test             | AC    | Time  |
|------------------|-------|-------|
| 01 Diagnostic    | OK    | 15:26 |
| 02 Room Air      | 0.000 | 15:26 |
| 03 *Subject Test | RFI*  | 15:28 |
| 04 Room Air      | 0.000 | 15:28 |

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 14323080A1  
Cyl No = 69  
Expiration Date = 06/05/2025  
County = 08      Oper No. = 133237

I followed the Approved Method and the  
instructions displayed by the Intoxilyzer  
in conducting this test.

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:29

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 15:30 |
| 02 Std. Gas | 0.081 | 15:30 |
| 03 Room Air | 0.000 | 15:31 |
| 04 Std. Gas | 0.080 | 15:31 |
| 05 Room Air | 0.000 | 15:32 |
| 06 Std. Gas | 0.080 | 15:32 |
| 07 Room Air | 0.000 | 15:33 |

Lot No = 14323080A1  
Cyl No = 69  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:33

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 15:34 |
| 02 Std. Gas | 0.081 | 15:34 |
| 03 Room Air | 0.000 | 15:35 |
| 04 Std. Gas | 0.080 | 15:35 |
| 05 Room Air | 0.000 | 15:36 |
| 06 Std. Gas | 0.080 | 15:36 |
| 07 Room Air | 0.000 | 15:36 |

Lot No = 14323080A1  
Cyl No = 69  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry Cal check #4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = TOXL      8164.14.00 09/16  
04/04/2025      15:37

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 15:38 |
| 02 Std. Gas | 0.081 | 15:38 |
| 03 Room Air | 0.000 | 15:39 |
| 04 Std. Gas | 0.081 | 15:39 |
| 05 Room Air | 0.000 | 15:40 |
| 06 Std. Gas | 0.080 | 15:40 |
| 07 Room Air | 0.000 | 15:41 |

Lot No = 14323080A1  
Cyl No = 69  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000