



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 5939

Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
  - Gas Cylinder Yes or No (If Yes, Lot # 01524080A4 Cyl. # 37)
  - Keys Yes or No
  - Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: WILL
5. ☒ Battery Check
  - Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
  - Replaced Simulator O-Ring Yes or No
  - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
  - Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
  - Display: 502 psi Regulator: 500 psi
  - Display and Regulator  $\pm$  50 psi of each other Yes or No
  - Gas tank tare necessary? Yes or No
  - If Yes, display readings after tare (Level 3,M,C,G):
  - Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
  - Wet Calibration Check - Low AC (Level 1,C)
  - Known Value  $\leq$  0.03 AC: 0.020 AC
  - Sim. Ser #: MP5321
  - Lot #: 202311D
  - Exp. Date: 11/28/25
  - ☒ Results  $\pm$  0.005 of known AC

2. ☒ Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - High AC (Level 1,C)  
Known Value  $\geq 0.25$  AC: 0.300 AC  
Sim. Ser #: MP6035  
Lot #: 202402C  
Exp. Date: 2/14/26  
☒ Results  $\pm 5\%$  AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).  
Known Value : 0.080 AC  
Gas Cylinder Lot #: 14323080A1  
Cylinder #: 7a  
Exp. Date: 6/5/25
4. ☒ Interferent Check (Level 1,B)  
Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR7352  
Lot #: ICS8  
Exp. Date: None  
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)  
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)  
Test 1 0.079 Test 4 0.079 Test 7 0.080  
Test 2 0.080 Test 5 0.079 Test 8 0.079  
Test 3 0.079 Test 6 0.079 Test 9 0.080  
Average 0.079  
☒ Results  $\pm 0.005$  AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

Ann Meel  
Inspector Signature

27 MAY 2025  
Date

Janelle Putschker  
Reviewer

28 May 2025  
Date

CMI, Inc. Intoxilyzer	Alcohol Analyzer
North Dakota Model 8000	SN 80-005939
Location = TOXL	8164.14.00 09/16
05/27/2025	10:31

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005939  
Location = TOXL      8164.14.00 09/16  
05/27/2025      10:32

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:33
02 Std. Sol.	0.021	10:34
03 Room Air	0.000	10:35
04 Std. Sol.	0.021	10:35
05 Room Air	0.000	10:36
06 Std. Sol.	0.020	10:37
07 Room Air	0.000	10:37

08 Sim Temp = 34.0°C

Simul Ser No = MP5321  
Std Sol No = 202311D  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: LOW AC Check - 0.020 AC

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005939  
Location = TOXL      8164.14.00 09/16  
05/27/2025      12:43

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:44
02 Std. Sol.	0.293	12:45
03 Room Air	0.000	12:45
04 Std. Sol.	0.295	12:46
05 Room Air	0.000	12:46
06 Std. Sol.	0.296	12:47
07 Room Air	0.000	12:48


08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: High AC Check - 0.300AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005939  
Location = TOXL      8164.14.00 09/16  
05/27/2025      12:49

Test	AC	Time
01 Room Air	0.000	12:49
02 *Subject Test	INT*	12:50
03 Room Air	0.000	12:50

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = INTERFERENT CK  
Dr. Lic. = ND/TES989643  
Lot No = 14323080A1  
Cyl No = 72  
Expiration Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Interferent check  
0.10AC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005939  
Location = TOXL      8164.14.00 09/16  
05/27/2025      12:51

Test	AC	Time
01 Diagnostic	OK	12:51
02 Room Air	0.000	12:52
03 *Subject Test	RFI*	12:52
04 Room Air	0.000	12:53

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 14323080A1  
Cyl No = 72  
Expiration Date = 06/05/2025  
County = 08      Oper No. = 133237

I followed the Approved Method and the  
instructions displayed by the Intoxilyzer  
in conducting this test.

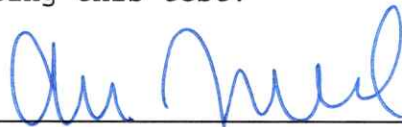

Operator Signature  
ANNA NAREHOOD

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005939  
Location = TOXL      8164.14.00 09/16  
05/27/2025      12:53

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:54
02 Std. Gas	0.079	12:54
03 Room Air	0.000	12:54
04 Std. Gas	0.080	12:55
05 Room Air	0.000	12:55
06 Std. Gas	0.079	12:56
07 Room Air	0.000	12:56

Lot No = 14323080A1  
Cyl No = 72  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005939  
Location = TOXL      8164.14.00 09/16  
05/27/2025      12:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:57
02 Std. Gas	0.079	12:58
03 Room Air	0.000	12:58
04 Std. Gas	0.079	12:59
05 Room Air	0.000	12:59
06 Std. Gas	0.079	13:00
07 Room Air	0.000	13:00

Lot No = 14323080A1  
Cyl No = 72  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005939  
Location = TOXL      8164.14.00 09/16  
05/27/2025      13:01

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:02
02 Std. Gas	0.080	13:02
03 Room Air	0.000	13:02
04 Std. Gas	0.079	13:03
05 Room Air	0.000	13:03
06 Std. Gas	0.080	13:04
07 Room Air	0.000	13:04

Lot No = 14323080A1  
Cyl No = 72  
Exp Date = 06/05/2025  
County = 08      Oper No. = 133237



Operator Signature  
ANNA NAREHOOD

Remarks: Dry cal check #7-9

Form 106-I8000