

**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

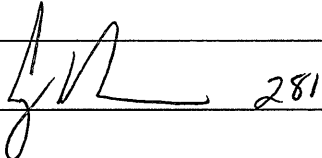
CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59281 (06/2018)

Serial Number 80-005939	Instrument Location Williston PD
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	


Check When Done:

- ☒ 1. Surge Protector Installed/Property Grounded.
- ☒ 2. Telephone Line Connected to Intoxilyzer® 8000.
- ☒ 3. Breath Tube Heated.
- ☒ 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- ☒ 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- ☒ 6. Run Tests:
 - ☒ A. Print Test (Level 1, Function P).
 - ☒ B. ACA Test (Level 1, Function C).
 - ☒ C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- ☐ 7. Repair and/or Maintenance Performed (if any): _____
- ☒ 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- ☒ 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- ☒ 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature  281	Date 5/31/2025
--	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By Anna Narehood 	Certified Date 09June2025
--	-------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = WILL 8164.14.00 09/16
05/31/2025 09:36

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$%^&*()_+?

Current Instrument Setup

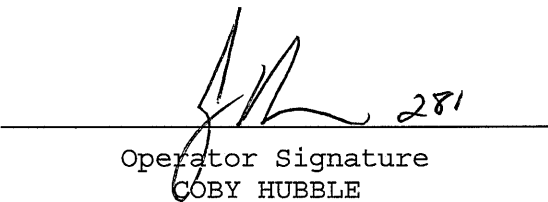
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01524080A4
Standard Cyl #? 37
Standard Expiration? 03/05/2026
Oper No? 030922

Flow Cal. Date: 06/18/2020
Slope 611
Intercept -592495

IR Calibration Date: 06/18/2020
 3um 9um

0th Coef(*100):	-15726	-19510
1st Coef(*100):	296627	143165
2nd Coef(*100):	-369	494
H2O adj(mg/l*10k):	220	240

***** Printer Test End *****


Operator Signature
COBY HUBBLE

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = WILL 8164.14.00 09/16
05/31/2025 09:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:38
02 Std. Gas	0.079	09:38
03 Room Air	0.000	09:39
04 Std. Gas	0.078	09:39
05 Room Air	0.000	09:39
06 Std. Gas	0.079	09:40
07 Room Air	0.000	09:40

Lot No = 01524080A4
Cyl No = 37
Exp Date = 03/05/2026
County = 53 Oper No. = 030922


Operator Signature
COBY HUBBLE

Remarks:

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = WILL 8164.14.00 09/16
05/31/2025 09:45

Test	AC	Time
01 Room Air	RFI*	09:48
02 Room Air	0.000	09:49

*Invalid Test
Inhibited - RFI

Sub Name = RFI TEST, NA NA
Sub DOB = 01/01/2000
Sub Sex = Male Weight = NA
Test = OTH Cit = NA
Dr. Lic. = ND/NA
Lot No = 01524080A4
Cyl No = 37
Expiration Date = 03/05/2026
County = 53 Oper No. = 030922



Operator Signature
COBY HUBBLE

Remarks:

Form 106-I8000