



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4199 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # _____ Cyl. # _____)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: TOXL
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 960 psi Regulator: 950 psi
Display and Regulator $\pm$ 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value $\leq$ 0.03 AC: 0.020 AC
Sim. Ser #: MP5321
Lot #: 202311D
Exp. Date: 11/28/25
☒ Results $\pm$ 0.005 of known AC

2. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - High AC (Level 1,C)
Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP6035
Lot #: 202402C
Exp. Date: 2/14/26
☒ Results $\pm 5\%$ AC of known AC
3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).
Known Value : 0.080 AC
Gas Cylinder Lot #: 28423080A3
Cylinder #: 41
Exp. Date: 11/5/25
4. ☒ Interferent Check (Level 1,B)
Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7352
Lot #: 1CS8
Exp. Date: None
☒ Display reads "Interferent Detect"
5. ☒ RFI Check (CMS Mode)
☒ Display reads "RFI Detect"
6. ☒ Dry Calibration Check (Level 1,C)
- | | | |
|----------------------|---------------------|---------------------|
| Test 1 <u>0.076</u> | Test 4 <u>0.078</u> | Test 7 <u>0.078</u> |
| Test 2 <u>0.078</u> | Test 5 <u>0.078</u> | Test 8 <u>0.077</u> |
| Test 3 <u>0.077</u> | Test 6 <u>0.078</u> | Test 9 <u>0.079</u> |
| Average <u>0.077</u> | | |
- ☒ Results ± 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

[Signature]
Inspector Signature

06 June 2025
Date

[Signature]
Reviewer

07 June 2025
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 10:55

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01524080A4
Standard Cyl #? 31
Standard Expiration? 03/05/2026
Oper No? 133237

Flow Cal. Date: 06/17/2019
Slope 593
Intercept -481610

IR Calibration Date: 04/18/2024
 3um 9um

0th Coef(*100):	-25088	-28296
1st Coef(*100):	269537	131183
2nd Coef(*100):	2308	1373
H2O adj(mg/l*10k):	357	563

***** Printer Test End *****


Operator Signature
ANNA NAREHOOD

Remarks: print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 15:02

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:03
02 Std. Sol.	0.017	15:04
03 Room Air	0.000	15:04
04 Std. Sol.	0.016	15:05
05 Room Air	0.000	15:05
06 Std. Sol.	0.017	15:06
07 Room Air	0.000	15:07

08 Sim Temp = 34.0°C

Simul Ser No = MP5321

Std Sol No = 202311D

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks:

Low AC check - 0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:34
02 Std. Sol.	0.295	11:36
03 Room Air	0.000	11:36
04 Std. Sol.	0.296	11:37
05 Room Air	0.000	11:38
06 Std. Sol.	0.297	11:38
07 Room Air	0.000	11:39


08 Sim Temp = 34.0°C

Simul Ser No = MP6035

Std Sol No = 202402C

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High calibration check - 0.300Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:42

Test	AC	Time
01 Room Air	0.000	11:43
02 *Subject Test	INT*	11:45
03 Room Air	0.000	11:45

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *interferent check*
0.10AC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 12:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	12:58
02 Room Air	0.000	12:58

*Invalid Test
Inhibited - RFI

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237

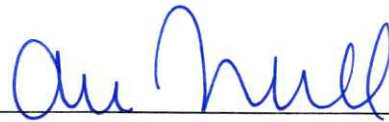

Operator Signature
ANNA NAREHOOD

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 14:00

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:01
02 Std. Gas	0.076	14:01
03 Room Air	0.000	14:02
04 Std. Gas	0.078	14:02
05 Room Air	0.000	14:03
06 Std. Gas	0.077	14:03
07 Room Air	0.000	14:04

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #1-3

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 14:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:10
02 Std. Gas	0.078	14:11
03 Room Air	0.000	14:11
04 Std. Gas	0.078	14:12
05 Room Air	0.000	14:12
06 Std. Gas	0.078	14:12
07 Room Air	0.000	14:13

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Dry cal check #4-6

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 14:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:14
02 Std. Gas	0.078	14:15
03 Room Air	0.000	14:15
04 Std. Gas	0.077	14:15
05 Room Air	0.000	14:16
06 Std. Gas	0.079	14:16
07 Room Air	0.000	14:17

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: dry cal check #7-9

Form 106-I8000