



**NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION**

INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4199

A. General Setup and Checks:

1. Initial start up
 - ☒ Power On
 - ☒ 5-minute countdown during initial warm-up
 - ☒ 1-minute countdown to begin test after standby mode
2. ☒ Display Intensity (Ctrl + ↑ or ↓)
3. Password Security:
 - ☒ Level 1 (Operator)
 - ☒ Level 2 (Field Inspector)
 - ☒ Level 3 (Lab Personnel)
4. ☒ Printer Setup (Level 3,S,P)
5. ☒ Forms Load Completed (CMI, Inc., CoBrA Software)

B. Level 1 Setup and Checks:

1. ☒ Internal Printer Test (Level 1,P). Sign and attach record.
 - ☒ Paper Feed
2. ☒ External Printer Test (Level 1,P). Sign and attach record.
3. Barcode Reader (Level 1,B) (Tone sounds after each)
 - ☒ Operator ID
 - ☒ Invalid ID
 - ☒ ND License
 - ☒ R key: Refusal. Sign and attach record.

C. Level 2 Setup and Checks:

1. ☒ Continuous Air Blank (Level 2,A)
2. ☒ Diagnostic (Level 2,D). Sign and attach test record.
3. ☒ Prelim Data Entry (Level 2,E)
4. Ser Number/Version Info (Level 2,V):

Inst Ser#: <u>80-004199</u>	DSP Ver: <u>1302.14</u>
Core Ver: <u>8164.14</u>	CPLD Ver: <u>7</u>

D. Level 3 Setup and Checks:

1. DVM Monitor (Level 3,D,D):

3: 12279 s: 1 C: 47.00
9: 12144 s: 1 B: 45

☒ DVM (3 & 9) between 9,000-16,000 counts

☒ RFI indicator with keyed radio: 0 → 1

2. Function (F) Keys:

☒ F5 – Tone

☒ F9 - Fan

☒ F6 – Green LED

☒ F10 – Pump

☒ F7 – Red LED

☒ F11 – Solenoid

3. Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 958 CF: 1.05

4. Flow Monitor (Level 3,D,F): Flow Sensor, R: 79 F: 0.000 L/s

5. Temperature Monitor (Level 3,D,T):

C: 47.0 A: 47.5 I: 0.0

B: 44.9 V: 0.0

☒ Cell Temperature (C) between 47 ± 0.02 °C

☒ Breath Hose Temperature (B) between 35.5 – 47 °C

☒ Internal Ambient Temperature (A) above 41 °C

6. Tank Monitor (Level 3,D,G):

Display: 960 psi Regulator: 950 psi

Display and Regulator ± 50 psi of each other Yes or No

Gas tank tare necessary? Yes or No

If Yes, display readings after tare (Level 3,M,C,G):

Display: _____ psi Regulator: _____ psi

7. ☒ General Setup (Level 3,S,G)

8. ☒ Configure Start Test (Level 3,S,T)

9. ☒ Network (Level 3,S,N)

E. Tests (Sign and attach all test records):

1. ☒ Configure wet bath simulator for the following test (Level 1,S)

Zero AC-Wet Calibration Check (Level 1,C):

Sim ser #: MP3003 Lot #: N/A Exp date: N/A

Known value: 0.000 AC

☒ Results are Zero AC

2. ☒ Configure wet bath simulator for the following test (Level 1,S)

Low AC-Wet Calibration Check (Level 1,C):

Known Value ≤ 0.03 AC: 0.020 AC


Sim ser #: MP532-1 Lot #: 202311D Exp date: 11/28/25

☒ Results ± 0.005 of known AC


3. ☒ Configure wet bath simulator for the following test (Level 1,S)
 High AC-Wet Calibration Check (Level 1,C):
 Known Value $\geq$ 0.25 AC: 0.300 AC
 Sim ser #: MPV035 Lot #: 202402C Exp date: 2/14/26
☒ Results $\pm$ 5% of known AC
4. ☒ Configure dry gas standard for the following tests (Level 1,S)
 Known Value: 0.080 AC
 Gas Cylinder Lot #: 28423080A3 Cylinder #: 41 Exp. Date: 11/5/25
5. 0.10% Ethanol + 0.05% Acetone (Level 1,B):
 Sim. Ser #: MPDR7352 Lot #: ICS 8 Exp. Date: None
☒ Display reads "Interferent Detect"
6. 0.05% Acetone (Level 1,B):
 Sim. Ser #: DR7111 Lot #: AC-ACE4 Exp. Date: None
☒ Display reads "Interferent Detect"
7. 0.10% Methanol (Level 1,B):
 Sim. Ser #: DR7345 Lot #: MET4 Exp. Date: None
☒ Display Reads "Interferent Detect"
8. 0.10% Isopropanol (Level 1,B):
 Sim. Ser #: DR7350 Lot #: IPA4 Exp. Date: None
☒ Display Reads "Interferent Detect"
9. ☒ Ambient Fail (Level 1,B): Display read and test record correct.
10. ☒ Invalid Sample (Level 1,B): Display read and test record correct.
11. ☒ Sequence Aborted (Level 1,B): Display read and test record correct.
12. ☒ ABA (Level 1,B): Test record correct.
13. ☒ Calibration check out of tolerance (CMS mode): Display read and test record correct.
14. ☒ RFI Detected (B,C, or CMS mode): Display read and test record correct.
15. ☒ Tank Pressure Below Minimum (CMS mode): Display reads correct.
16. ☒ Deficient Samples (CMS mode): Display read and test record correct.
17. ☒ Improper Sample (CMS mode): Display read and test record correct.
18. ☒ Difference Too Great (CMS mode): Display read and test record correct.
19. ☒ CMS (CMS mode): Test record correct.
20. Stability Test (Level 3,T,S):
 Ave: 0.0775 Std Dev: 0.0005 Rel Std Dev: 0.106

Maintenance/Repairs/Notes: NIA

Instrument is acceptable to be used in the field. Yes or No
If No, state reason(s) why:


Inspector Signature

06 June 2025
Date


Reviewer

07 June 2025
Date

Intoxilyzer Test Record and Checklist
NDORS Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/16/2025 14:20

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHJKLM

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMN

24 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMN

32 characters per line
abcdefghijklmnopqrstuwx123456
ABCDEFGHIJKLMN

42 characters per line
abcdefghijklmnopqrstuwx1234567890abcdef
ABCDEFGHIJKLMN

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 28423080A3
Standard Cyl #? 41
Standard Expiration? 11/05/2025
Oper No? 133237

Flow Cal. Date: 06/17/2019
Slope 593
Intercept -481610

IR Calibration Date: 04/18/2024
3um 9um

0th Coef(*100):	-25088	-28296
1st Coef(*100):	269537	131183
2nd Coef(*100):	2308	1373
H2O adj(ng/1*10k):	357	563

***** Test End *****



Operator Signature
ANNA NAREHOOD

Remarks:

Internal Print
Test

Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 10:55

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 01524080A4
Standard Cyl #? 31
Standard Expiration? 03/05/2026
Oper No? 133237

Flow Cal. Date: 06/17/2019
Slope 593
Intercept -481610

IR Calibration Date: 04/18/2024
 3um 9um

0th Coef(*100):	-25088	-28296
1st Coef(*100):	269537	131183
2nd Coef(*100):	2308	1373
H2O adj(mg/l*10k):	357	563

***** Printer Test End *****

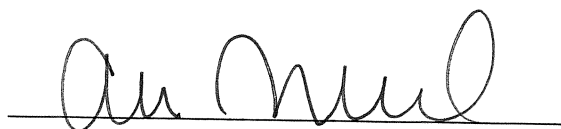

Operator Signature
ANNA NAREHOOD

Remarks: External Print Test


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 10:55

Test	AC	Time
01 Room Air	0.000	10:56
02 *Subject Test	REF*	10:56
03 Room Air	0.000	10:57

*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = REFUSAL
Dr. Lic. = ND/DIS821456
Lot No = 01524080A4
Cyl No = 31
Expiration Date = 03/05/2026
County = 08 Oper No. = 133237

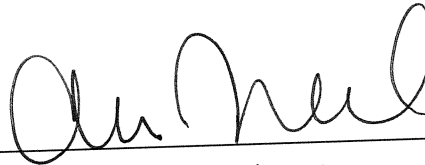

Operator Signature
ANNA NAREHOOD

Remarks:

Refusal

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:01

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 133237

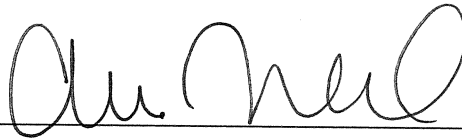

Operator Signature
ANNA NAREHOOD

Remarks: Diagnostic

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:07

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:08
02 Std. Sol.	0.000	11:09
03 Room Air	0.000	11:09
04 Std. Sol.	0.000	11:10
05 Room Air	0.000	11:10
06 Std. Sol.	0.000	11:11
07 Room Air	0.000	11:12

08 Sim Temp = 34.0°C

Simul Ser No = MP3003

Std Sol No = NA

County = 08

Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Zero AC cal check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 15:02

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:03
02 Std. Sol.	0.017	15:04
03 Room Air	0.000	15:04
04 Std. Sol.	0.016	15:05
05 Room Air	0.000	15:05
06 Std. Sol.	0.017	15:06
07 Room Air	0.000	15:07

08 Sim Temp = 34.0°C

Simul Ser No = MP5321
Std Sol No = 202311D
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: LOW AC CHECK - 0.020AR

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:34
02 Std. Sol.	0.295	11:36
03 Room Air	0.000	11:36
04 Std. Sol.	0.296	11:37
05 Room Air	0.000	11:38
06 Std. Sol.	0.297	11:38
07 Room Air	0.000	11:39

08 Sim Temp = 34.0°C

Simul Ser No = MP6035
Std Sol No = 202402C
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: High AC check - 0.300AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:42

Test	AC	Time
01 Room Air	0.000	11:43
02 *Subject Test	INT*	11:45
03 Room Air	0.000	11:45

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent check
0.10Ac + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:46

Test	AC	Time
01 Room Air	0.000	11:47
02 *Subject Test	INT*	11:47
03 Room Air	0.000	11:48

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = INTERFERENT ACE
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: 0.05% Acetone
Interferent check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:49

Test	AC	Time
01 Room Air	0.000	11:50
02 *Subject Test	INT*	11:50
03 Room Air	0.000	11:51

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = INTERFERENT MET
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks:

interferent check
0.10% Methanol

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:51

Test	AC	Time
01 Room Air	0.000	11:52
02 *Subject Test	INT*	11:52
03 Room Air	0.000	11:53

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = INTERFERENT IPA
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Interferent check
0.10% Isopropanol

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:53

Test	AC	Time
01 Room Air	AMB*	11:54
02 Room Air	PUR**	11:55

*Invalid Test
Check Ambient Conditions
**Purge Fail

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = AMBIENT FAIL
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks:
Ambient Fail

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 11:57

Test	AC	Time
01 Room Air	0.000	11:58
02 Invalid Sample	X.XXX	11:58
03 Room Air	0.000	11:59

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = INVALID SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: Invalid Sample

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 12:45

Test	AC	Time
01 Room Air	ABT*	12:45
02 Room Air	0.000	12:46

*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = SEQUENCE ABORT
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: *Sequence Aborted*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 12:48

Test	AC	Time
01 Room Air	0.000	12:48
02 Subject Test 1	0.000	12:49
03 Room Air	0.000	12:49
04 Reported AC	0.000	12:49

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = ABA TEST
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237



Operator Signature
ANNA NAREHOOD

Remarks: ABA Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 12:51

Test	AC	Time
01 Diagnostic	OK	12:52
02 Room Air	0.000	12:53
03 Subject Test 1	0.000	12:53
04 Room Air	0.000	12:55
05 Std. Gas	0.000*	12:57
06 Room Air	0.000	12:57

*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = CAL CHECK OOT
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: Calibration check out of
tolerance

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 12:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	12:58
02 Room Air	0.000	12:58

*Invalid Test
Inhibited - RFI

Lot No = 28423080A3
Cyl No = 41
Exp Date = 11/05/2025
County = 08 Oper No. = 133237

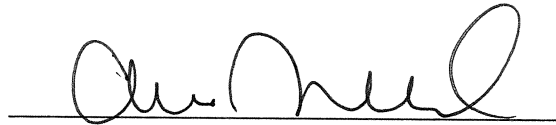

Operator Signature
ANNA NAREHOOD

Remarks: RFI Detected

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 12:59

Test	AC	Time
01 Diagnostic	OK	13:00
02 Room Air	0.000	13:01
03 *Subject Test	0.000*	13:04
04 Room Air	0.000	13:06
05 Std. Gas	0.078	13:07
06 Room Air	0.000	13:08
07 *Subject Test	0.000*	13:12
08 Room Air	0.000	13:12

No RFI Detected

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = DEFICIENT SAMPL
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: Deficient Samples

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 13:13

Test	AC	Time
01 Diagnostic	OK	13:14
02 Room Air	IPS*	13:14
03 Room Air	0.000	13:14

*Improper Sample

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = IMPROPER
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: Improper sample

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 13:14

Test	AC	Time
01 Diagnostic	OK	13:15
02 Room Air	0.000	13:16
03 Subject Test 1	0.098*	13:16
04 Room Air	0.000	13:19
05 Std. Gas	0.078	13:20
06 Room Air	0.000	13:21
07 Subject Test 2	0.000*	13:22
08 Room Air	0.000	13:27

*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = DIFF TOO GREAT
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA NAREHOOD

Remarks: Difference too Great

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 13:31

Test	AC	Time
01 Diagnostic	OK	13:32
02 Room Air	0.000	13:33
03 Subject Test 1	0.000	13:33
04 Room Air	0.000	13:36
05 Std. Gas	0.078	13:37
06 Room Air	0.000	13:38
07 Subject Test 2	0.000	13:39
08 Room Air	0.000	13:40
09 Reported AC	0.000	13:33

Difference OK
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = OTH Cit = CMS TEST
Dr. Lic. = ND/DIS821456
Lot No = 28423080A3
Cyl No = 41
Expiration Date = 11/05/2025
County = 08 Oper No. = 133237

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.


Operator Signature
ANNA NAREHOOD

Remarks: CMS Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = TOXL 8164.14.00 09/16
06/06/2025 13:40

Test	AC	Time
01 Room Air	0.000	13:41
02 Std. Gas	0.077	13:41
03 Room Air	0.000	13:42
04 Std. Gas	0.077	13:42
05 Room Air	0.000	13:43
06 Std. Gas	0.077	13:43
07 Room Air	0.000	13:44
08 Std. Gas	0.077	13:44
09 Room Air	0.000	13:44
10 Std. Gas	0.078	13:45
11 Room Air	0.000	13:45
12 Std. Gas	0.078	13:46
13 Room Air	0.000	13:46
14 Std. Gas	0.077	13:46
15 Room Air	0.000	13:47
16 Std. Gas	0.077	13:47
17 Room Air	0.000	13:48
18 Std. Gas	0.077	13:48
19 Room Air	0.000	13:49
20 Std. Gas	0.078	13:49
21 Room Air	0.000	13:50
22 Std. Gas	0.078	13:50
23 Room Air	0.000	13:51
24 Std. Gas	0.077	13:51
25 Room Air	0.000	13:51
26 Std. Gas	0.077	13:52
27 Room Air	0.000	13:52
28 Std. Gas	0.077	13:53
29 Room Air	0.000	13:53
30 Std. Gas	0.078	13:53
31 Room Air	0.000	13:54
32 Std. Gas	0.077	13:54
33 Room Air	0.000	13:55
34 Std. Gas	0.078	13:55
35 Room Air	0.000	13:56
36 Std. Gas	0.078	13:56
37 Room Air	0.000	13:57
38 Std. Gas	0.078	13:57
39 Room Air	0.000	13:57
40 Std. Gas	0.078	13:58
41 Room Air	0.000	13:58
42 Cal Check Stats:		
43 Average	0.0775	
44 Std Dev	0.0005	
45 Rel Std Dev	0.66%	


Handwritten signature
06 June 2025
AEN

Operator Signature
ANNA NAREHOOD

Remarks:

Stability Test

Form 106-I8000

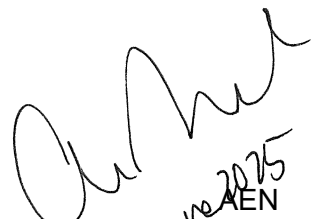
06 June 2025
AEN