



# ETHANOL GAS STANDARD CYLINDER REPORT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59282 (08/2018)

Chemical Test Operator Name (Print) Michael Dehn		
Location Divide County Sheriff's Department		Intoxilyzer® Serial Number 80-006682
Gas Lot Number 25024080A3	Gas Cylinder Number 001	Gas Expiration Date 10/05/2026

Check When Done:

- ☒ 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- aen* ☒ 2. Perform an ACA Test (Level 1, Function C).  
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).  
A. 0.081 AC  
B. 0.082 AC  
C. 0.080 AC
- ☒ 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- ☒ 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- ☒ 5. Send the Following to the Crime Laboratory:  
A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).  
B. ACA Test Record.

Chemical Test Operator Signature <i>Michael Dehn</i>	Date 08/07/2025
Reviewed By (Crime Laboratory Use Only) <i>Anna Narehood</i>	Date 8/8/2025

The undersigned, having custody of the original record, certifies that the information hereon is a true and correct copy of the original document maintained as part of the activities of this office.

*Michael Dehn*  
Signature

*08/07/25*  
Date

The gas lot number found on the three test records from the installation and Repair checkout (104-G) dated April 29, 2025 listed an incorrect lot number for the gas cylinder. The gas tank lot number (232442) was accidentally used instead of the correct gas cylinder lot instead of the correct gas cylinder lot number of 25024080A3. A new ethanol gas standard cylinder report with the corrected gas cylinder lot number dated August 7, 2025 is attached. ~~These~~ Tests run with the incorrect gas cylinder lot number are still valid tests.

FORM 105-G

AEN 8/8/2025

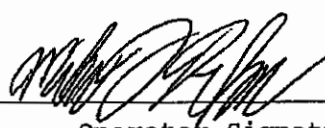
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006682  
Location = CROS      8164.14.00 09/16  
08/07/2025      10:54

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:55
02 Std. Gas	0.081	10:55
03 Room Air	0.000	10:55
04 Std. Gas	0.080	10:56
05 Room Air	0.000	10:56
06 Std. Gas	0.080	10:57
07 Room Air	0.000	10:57

Lot No = 25024080A3  
Cyl No = 1  
Exp Date = 10/05/2026  
County = 12      Oper No. = 130831

  
Operator Signature  
MICHAEL DEHN

Remarks:

Form 106-I8000

The undersigned, having custody of the  
original record, certifies that the information  
hereon is a true and correct copy of the  
original and is maintained as part of the  
activity log of the device.

  
Signature

08/07/25  
Date



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
SFN 59281 (06/2018)

Serial Number <b>80-006682</b>	Instrument Location <b>CRS</b>
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- ☒ 1. Surge Protector Installed/Property Grounded.
- ☒ 2. Telephone Line Connected to Intoxilyzer® 8000.
- ☒ 3. Breath Tube Heated.
- ☒ 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- ☒ 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- ☒ 6. Run Tests:
  - ☒ A. Print Test (Level 1, Function P).
  - ☒ B. ACA Test (Level 1, Function C).
  - ☒ C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- ☒ 7. Repair and/or Maintenance Performed (If any): \_\_\_\_\_
- ☐ 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place It by the Intoxilyzer® for Use.
- ☒ 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- ☐ 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date <b>4-29-25</b>
-------------------------------	------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <b>Anna Narehood</b>	Certified Date <b>30 April 2025</b>
---	--

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006682  
Location = CROS      8164.14.00 09/16  
04/29/2025      22:34

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-=  
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-=  
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&\*()\_+?

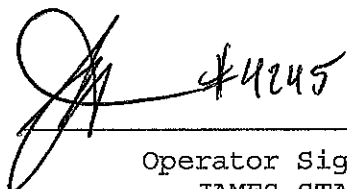
Current Instrument Setup

Data Entry Mode:      Enabled  
Start Test Sequence:      DABACABA  
Display Prelim Rslt?      Yes  
Display Third Digit?      Yes  
Inhib Printer(Y/N)?      No  
Display Volume?      No  
Disable On Memfull?      Yes  
# of Print Copies?      1  
Select Std (D/W/I)?      Dry  
Standard Value?      0.080  
Standard Lot #?      232492  
Standard Cyl #?      1  
Standard Expiration?      10/05/2026  
Oper No?      134037  
  
Flow Cal. Date:      09/06/2016  
Slope      701  
Intercept      -706193

IR Calibration Date:      09/06/2016  
   3um      9um

0th Coef(*100):	-17150	-23247
1st Coef(*100):	271726	134617
2nd Coef(*100):	831	1215
H2O adj(mg/l*10k):	393	518

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
Operator Signature  
JAMES STACEY

Remarks:      Printer Test.

Form 106-I8000

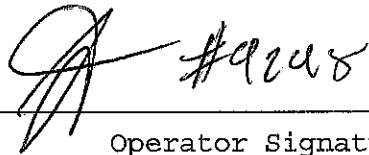
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006682  
Location = CROS      8164.14.00 09/16  
04/29/2025      22:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	22:42
02 Std. Gas	0.082	22:43
03 Room Air	0.000	22:43
04 Std. Gas	0.081	22:44
05 Room Air	0.000	22:44
06 Std. Gas	0.081	22:45
07 Room Air	0.000	22:45

Lot No = 232492  
Cyl No = 1  
Exp Date = 10/05/2026  
County = 12      Oper No. = 134037



Operator Signature  
JAMES STACEY

Remarks:

Form 106-I8000

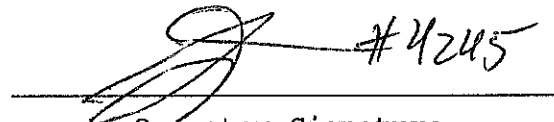
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006682  
Location = CROS      8164.14.00 09/16  
04/29/2025      22:46

Test	AC	Time
01 Room Air	0.000	22:48
02 *Subject Test	RFI*	22:49
03 Room Air	0.000	22:49

\*Invalid Test  
Inhibited - RFI

Sub Name = DUMMY, DUMMY L  
Sub DOB = 09/09/2000  
Sub Sex = Male      Weight = 230  
Test = OTH      Cit = 1  
Dr. Lic. = ND/NA  
Lot No = 232492  
Cyl No = 1  
Expiration Date = 10/05/2026  
County = 12      Oper No. = 134037

  
Operator Signature  
JAMES STACEY

Remarks:

RFI

Form 106-I8000