



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 80-004939	Instrument Location BCCC
Reason for Install/Repair	
<input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) Install after crime lab maintenance	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): **N/A**
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature [Signature]	Date 2/17/26
--	---------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By Anna Ingemansen	[Signature]	Certified Date 18Feb2026
--	--------------------	---------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = BCCC 8164.14.00 09/16
02/17/2026 18:57

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

Current Instrument Setup

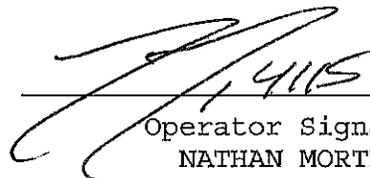
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer (Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 08425080A1
Standard Cyl #? 24
Standard Expiration? 05/05/2027
Oper No? 130095

Flow Cal. Date: 01/18/2010
Slope 724
Intercept -779308

IR Calibration Date: 06/22/2023

	3um	9um
0th Coef (*100):	-19230	-17600
1st Coef (*100):	257947	133671
2nd Coef (*100):	3268	1535
H2O adj (mg/l*10k):	529	419

***** Printer Test End *****


Operator Signature
NATHAN MORTEN

Remarks: *Print Test*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = BCCC 8164.14.00 09/16
02/17/2026 18:58

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:59
02 Std. Gas	0.084	18:59
03 Room Air	0.000	19:00
04 Std. Gas	0.082	19:00
05 Room Air	0.000	19:01
06 Std. Gas	0.083	19:01
07 Room Air	0.000	19:02

Lot No = 08425080A1
Cyl No = 24
Exp Date = 05/05/2027
County = 02 Oper No. = 130095


Operator Signature
NATHAN MORTEN

Remarks: *CAL check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

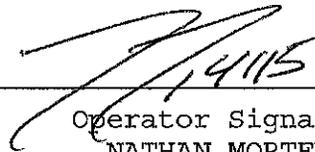
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = BCCC 8164.14.00 09/16
02/17/2026 19:03

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	19:03
02 Room Air	0.000	19:04

*Invalid Test
Inhibited - RFI

Lot No = 08425080A1
Cyl No = 24
Exp Date = 05/05/2027
County = 02 Oper No. = 130095


Operator Signature
NATHAN MORTEN

Remarks: RFI Test

Form 106-I8000