



# ETHANOL GAS STANDARD CYLINDER REPORT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59282 (08/2018)

Chemical Test Operator Name (Print) <i>Allen, Kathryn</i>		
Location <i>Cass Jail Booking</i>	Intoxilyzer® Serial Number <i>80-004206</i>	
Gas Lot Number <i>19825080 A2</i>	Gas Cylinder Number <i>35</i>	Gas Expiration Date <i>9-5-2027</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).  
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
  - A. *0.083* AC
  - B. *0.082* AC
  - C. *0.082* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
  - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
  - B. ACA Test Record.

Chemical Test Operator Signature <i>Kathryn Allen</i>	Date <i>3-1-2026</i>
Reviewed By (Crime Laboratory Use Only) <i>Anna Ingemansen</i> <i>Anna Ingemansen</i>	Date 04March2026

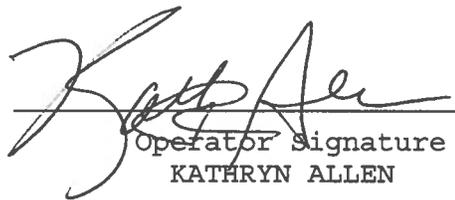
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004206  
Location = CASS      8164.14.00 09/16  
03/01/2026      16:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:16
02 Std. Gas	0.083	16:17
03 Room Air	0.000	16:17
04 Std. Gas	0.082	16:18
05 Room Air	0.000	16:18
06 Std. Gas	0.082	16:19
07 Room Air	0.000	16:19

Lot No = 19825080A2  
Cyl No = 35  
Exp Date = 09/05/2027  
County = 09      Oper No. = 090801

  
Operator Signature  
KATHRYN ALLEN

Remarks:  
New Canister Instal  
Form 106-I8000      All ok!