



ETHANOL GAS STANDARD CYLINDER REPORT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59282 (08/2018)

Chemical Test Operator Name (Print) <i>Allen Kathryn</i>		
Location <i>Cass County Jail Booking</i>	Intoxilyzer® Serial Number <i>80-004954</i>	
Gas Lot Number <i>19825080 A2</i>	Gas Cylinder Number <i>35</i>	Gas Expiration Date <i>9/5/2027</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
 Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 A. *0.077* AC
 B. *0.077* AC
 C. *0.077* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
 B. ACA Test Record.

Chemical Test Operator Signature <i>Kathy Allen</i>	Date <i>3-19-26</i>
Reviewed By (Crime Laboratory Use Only) <i>Anna Ingemansen</i>	Date <i>25Mar2026</i>

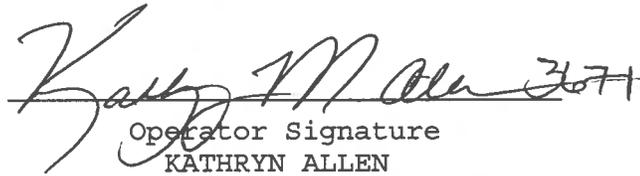
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004954
Location = CASS 8164.14.00 09/16
03/19/2026 16:53

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:54
02 Std. Gas	0.077	16:54
03 Room Air	0.000	16:54
04 Std. Gas	0.077	16:55
05 Room Air	0.000	16:55
06 Std. Gas	0.077	16:56
07 Room Air	0.000	16:56

Lot No = 19825080A2
Cyl No = 35
Exp Date = 09/05/2027
County = 09 Oper No. = 090801


Operator Signature
KATHRYN ALLEN

Remarks: Within Normal Range
New machine Installation
Form 106-I8000