

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 5950 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 19825080A2 Cyl. # 29)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: SHER
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 1000 psi Regulator: 1000 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.025 AC
Sim. Ser #: MP5290
Lot #: 202509A
Exp. Date: 10 Sept 27
 Results ± 0.005 of known AC
2. Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value \geq 0.25 AC: 0.300 AC

Sim. Ser #: MP5321

Lot #: 202408H

Exp. Date: 29 Aug 26

Results \pm 5% AC of known AC

3. Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 26-4437

Cylinder #: 104

Exp. Date: 1/29/28

4. Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: 1CS9

Exp. Date: None

Display reads "Interferent Detect"

5. Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6. RFI Check (CMS Mode)

Display reads "RFI Detect"

7. Dry Calibration Check (Level 1,C)

Test 1 0.081 Test 4 0.082 Test 7 0.081

Test 2 0.082 Test 5 0.082 Test 8 0.082

Test 3 0.082 Test 6 0.081 Test 9 0.081

Average 0.081

Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: Restarted instrument after High Cal. Check was printed on internal printer to establish connection with external printer.

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL.

[Signature]
Inspector Signature

02 April 2026
Date

[Signature]
Reviewer

07 Apr 2026
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = TOXL 8164.14.00 09/16
04/02/2026 14:07

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^&* () _ + ?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^&* () _ + ?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 19825080A2
Standard Cyl #? 29
Standard Expiration? 09/05/2027
Oper No? 133237

Flow Cal. Date: 06/20/2013
Slope 713
Intercept -723515

IR Calibration Date: 06/20/2013
 3um 9um

0th Coef(*100):	-37081	-23816
1st Coef(*100):	290549	133411
2nd Coef(*100):	552	1090
H2O adj(mg/l*10k):	683	502

***** Printer Test End *****

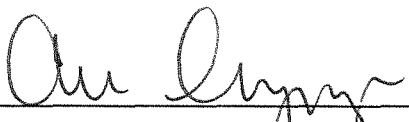

Operator Signature
ANNA INGEMANSEN

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = TOXL 8164.14.00 09/16
04/02/2026 14:08

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:09
02 Std. Sol.	0.025	14:09
03 Room Air	0.000	14:10
04 Std. Sol.	0.025	14:11
05 Room Air	0.000	14:11
06 Std. Sol.	0.025	14:12
07 Room Air	0.000	14:12


08 Sim Temp = 34.0°C

Simul Ser No = MP5290

Std Sol No = 202509A

County = 08

Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks:

Low Ac check
0.025Ac

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = TOXL 8164.14.00 09/16
04/02/2026 14:14

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:14
02 Std. Sol.	0.295	14:15
03 Room Air	0.000	14:16
04 Std. Sol.	0.296	14:17
05 Room Air	0.000	14:17
06 Std. Sol.	0.295	14:18
07 Room Air	0.000	14:18

08 Sim Temp = 34.0°C

Simul Ser No = MP5321
Std Sol No = 202408H
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks:
High AC Check
0.300AC

Form 106-18000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = TOXL 8164.14.00 09/16
04/02/2026 14:20

Test	AC	Time
01 Room Air	0.000	14:21
02 *Subject Test	INT*	14:21
03 Room Air	0.000	14:22

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 264437
Cyl No = 104
Expiration Date = 01/29/2028
County = 08 Oper No. = 133237

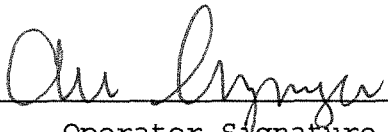

Operator Signature
ANNA INGEMANSEN

Remarks: Interferent check
0.10Ac + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = TOXL 8164.14.00 09/16
04/02/2026 14:25

Test	AC	Time
01 Room Air	0.000	14:26
02 Invalid Sample	X.XXX	14:26
03 Room Air	0.000	14:27

*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INVALID SAMPLE
Dr. Lic. = ND/TES989643
Lot No = 264437
Cyl No = 104
Expiration Date = 01/29/2028
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: Invalid sample
 Mouth alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = TOXL 8164.14.00 09/16
04/02/2026 14:27

Test	AC	Time
01 Diagnostic	OK	14:28
02 Room Air	0.000	14:29
03 *Subject Test	RFI*	14:29
04 Room Air	0.000	14:29

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 264437
Cyl No = 104
Expiration Date = 01/29/2028
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA INGEMANSEN

Remarks: RFI check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = TOXL 8164.14.00 09/16
04/02/2026 14:30

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:31
02 Std. Gas	0.081	14:31
03 Room Air	0.000	14:32
04 Std. Gas	0.082	14:32
05 Room Air	0.000	14:33
06 Std. Gas	0.082	14:33
07 Room Air	0.000	14:34


Lot No = 264437

Cyl No = 104

Exp Date = 01/29/2028

County = 08

Oper No. = 133237

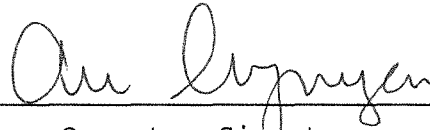

Operator Signature
ANNA INGEMANSEN

Remarks: Dry Cal Check
#1-3

Form 106-I8000

