



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 5945 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 08425080A1 Cyl. # 21)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: BSPD
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
 - Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
 - Display: 950 psi Regulator: 975 psi
 - Display and Regulator ± 50 psi of each other Yes or No
 - Gas tank tare necessary? Yes or No
 - If Yes, display readings after tare (Level 3,M,C,G):
 - Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
 - Wet Calibration Check - Low AC (Level 1,C)
 - Known Value ≤ 0.03 AC: 0.025 AC
 - Sim. Ser #: MP5290
 - Lot #: 202509A
 - Exp. Date: 10 sept 2027
 - Results ± 0.005 of known AC
2. Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value \geq 0.25 AC: 0.300 AC

Sim. Ser #: MP5321

Lot #: 202408H

Exp. Date: ~~29 Aug 2028~~ 29 Aug 2024 *aei 02Apr26*

Results \pm 5% AC of known AC

3. Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 19825080A2

Cylinder #: 20

Exp. Date: 9/5/2027

4. Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: ICS 9

Exp. Date: None

Display reads "Interferent Detect"

5. Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6. RFI Check (CMS Mode)

Display reads "RFI Detect"

7. Dry Calibration Check (Level 1,C)

Test 1 0.078 Test 4 0.079 Test 7 0.079

Test 2 0.078 Test 5 0.078 Test 8 0.079

Test 3 0.079 Test 6 0.078 Test 9 0.077

Average 0.078

Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL.

Am Lyngren
Inspector Signature

02 April 2026
Date

Janelle Pitschler
Reviewer

04 Apr. 2026
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:03

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 08425080A1
Standard Cyl #? 21
Standard Expiration? 05/05/2027
Oper No? 133237

Flow Cal. Date: 06/20/2013
Slope 637
Intercept -566407

IR Calibration Date: 05/22/2015

	3um	9um
0th Coef(*100):	-21213	-23093
1st Coef(*100):	279171	139292
2nd Coef(*100):	2898	1291
H2O adj(mg/l*10k):	332	319

***** Printer Test End *****



Operator Signature
ANNA INGEMANSEN

Remarks: *Print Test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:04

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:04
02 Std. Sol.	0.025	10:05
03 Room Air	0.000	10:06
04 Std. Sol.	0.025	10:06
05 Room Air	0.000	10:07
06 Std. Sol.	0.025	10:08
07 Room Air	0.000	10:08

08 Sim Temp = 34.0°C

Simul Ser No = MP5290
Std Sol No = 202509A
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: *LOW AC Check*
0.025AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:09

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:10
02 Std. Sol.	0.299	10:11
03 Room Air	0.000	10:12
04 Std. Sol.	0.301	10:12
05 Room Air	0.000	10:13
06 Std. Sol.	0.300	10:14
07 Room Air	0.000	10:14

08 Sim Temp = 34.0°C

Simul Ser No = MP5321
Std Sol No = 202408H
County = 08 Oper No. = 133237

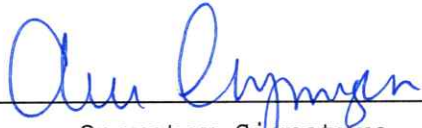

Operator Signature
ANNA INGEMANSEN

Remarks: High AC Check
= 0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:16

Test	AC	Time
01 Room Air	0.000	10:17
02 *Subject Test	INT*	10:18
03 Room Air	0.000	10:18

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 20
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: Interferent Check
0.10AC + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:19

Test	AC	Time
01 Room Air	0.000	10:21
02 Invalid Sample	X.XXX	10:21
03 Room Air	0.000	10:22

*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INVALID SAMPLE
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 20
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: Invalid sample
 -mouth alcohol

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:25

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:25
02 Std. Gas	0.078	10:26
03 Room Air	0.000	10:26
04 Std. Gas	0.078	10:27
05 Room Air	0.000	10:27
06 Std. Gas	0.079	10:27
07 Room Air	0.000	10:28

Lot No = 19825080A2
Cyl No = 20
Exp Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check
#1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:30

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:30
02 Std. Gas	0.079	10:31
03 Room Air	0.000	10:31
04 Std. Gas	0.078	10:32
05 Room Air	0.000	10:32
06 Std. Gas	0.078	10:33
07 Room Air	0.000	10:33

Lot No = 19825080A2
Cyl No = 20
Exp Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check
#4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = TOXL 8164.14.00 09/16
04/02/2026 10:33

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:34
02 Std. Gas	0.079	10:34
03 Room Air	0.000	10:35
04 Std. Gas	0.079	10:35
05 Room Air	0.000	10:36
06 Std. Gas	0.077	10:36
07 Room Air	0.000	10:37

Lot No = 19825080A2
Cyl No = 20
Exp Date = 09/05/2027
County = 08 Oper No. = 133237

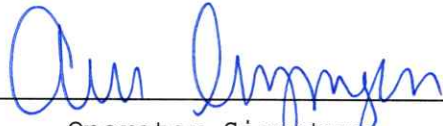

Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check
#7-9

Form 106-I8000