



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 6506 Inspection Location: MAND

A. Pre-Inspection

1. Items with Instrument:
  - Gas Cylinder Yes or No (If Yes, Lot # 25024080A3 Cyl. # 10)
  - Keys Yes or No
  - Power Cord Yes or No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: MAND
5.  Battery Check
  - Was the external battery pack replaced? Yes or No
6.  O-Rings
  - Replaced Simulator O-Ring Yes or No
  - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).  
Display: 946 psi Regulator: 950 psi  
Display and Regulator ± 50 psi of each other Yes or No  
Gas tank tare necessary? Yes or No  
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

1.  Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value ≤ 0.03 AC: 0.025 AC  
Sim. Ser #: MP3063  
Lot #: 202509A  
Exp. Date: 9/10/27  
 Results ± 0.005 of known AC
2.  Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value  $\geq$  0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

Results  $\pm$  5% AC of known AC

3.  Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 19825080A2

Cylinder #: 20

Exp. Date: 9/5/27

4.  Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: ICS9

Exp. Date: None

Display reads "Interferent Detect"

5.  Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6.  RFI Check (CMS Mode)

Display reads "RFI Detect"

7.  Dry Calibration Check (Level 1,C)

Test 1 0.081 Test 4 0.081 Test 7 0.081

Test 2 0.081 Test 5 0.081 Test 8 0.081

Test 3 0.081 Test 6 0.081 Test 9 0.081

Average 0.081

Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field.  Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL.

AW Dwyer  
Inspector Signature

08 April 2026  
Date

Janelle Postchiller  
Reviewer

10 Apr. 2026  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:10

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=-|  
ABCDEFGHIJKLMNPNOPQRSTUVWXYZ!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=-|  
ABCDEFGHIJKLMNPNOPQRSTUVWXYZ!@#%&^\*()\_+?

Current Instrument Setup

Data Entry Mode:      Enabled  
Start Test Sequence:      DABACABA  
Display Prelim Rslt?      Yes  
Display Third Digit?      Yes  
Inhib Printer(Y/N)?      No  
Display Volume?      No  
Disable On Memfull?      Yes  
# of Print Copies?      1  
Select Std (D/W/I)?      Dry  
Standard Value?      0.080  
Standard Lot #?      25024080A3  
Standard Cyl #?      10  
Standard Expiration?      10/05/2026  
Oper No?      133237

Flow Cal. Date:      08/20/2015  
Slope      657  
Intercept      -627881

IR Calibration Date:      08/20/2015

	3um	9um
0th Coef(*100):	-22470	-18919
1st Coef(*100):	266505	136109
2nd Coef(*100):	3702	1644
H2O adj(mg/l*10k):	709	510

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Print Test*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:13

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:14
02 Std. Sol.	0.027	10:15
03 Room Air	0.000	10:16
04 Std. Sol.	0.026	10:16
05 Room Air	0.000	10:17
06 Std. Sol.	0.026	10:18
07 Room Air	0.000	10:18

08 Sim Temp = 34.0°C

Simul Ser No = MP3063  
Std Sol No = 202509A  
County = 08      Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks:

~~Dry Cal Check~~ acj 4/8/26  
Low AC Check 0.025 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

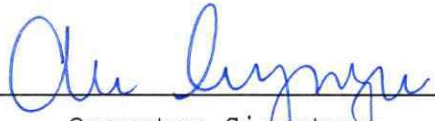
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:20

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:21
02 Std. Sol.	0.300	10:22
03 Room Air	0.000	10:23
04 Std. Sol.	0.301	10:24
05 Room Air	0.000	10:24
06 Std. Sol.	0.301	10:25
07 Room Air	0.000	10:25

08 Sim Temp = 34.0°C

Simul Ser No = MP3003  
Std Sol No = 202408H  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: High AC Check  
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:27

Test	AC	Time
01 Room Air	0.000	10:28
02 *Subject Test	INT*	10:28
03 Room Air	0.000	10:29

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = INTERFERENT CK  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08      Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Interferent check  
0.10AC + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:30

Test	AC	Time
01 Room Air	0.000	10:31
02 Invalid Sample	X.XXX	10:31
03 Room Air	0.000	10:32

\*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = INVALID  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08      Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks:

Invalid sample  
Mouth alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:35

Test	AC	Time
01 Diagnostic	OK	10:36
02 Room Air	0.000	10:36
03 *Subject Test	RFI*	10:37
04 Room Air	0.000	10:37

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08      Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: RFI Check

Form 106-I8000

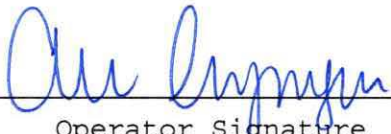
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:38

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:38
02 Std. Gas	0.081	10:39
03 Room Air	0.000	10:39
04 Std. Gas	0.081	10:39
05 Room Air	0.000	10:40
06 Std. Gas	0.081	10:40
07 Room Air	0.000	10:41

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
#1-3

Form 106-I8000

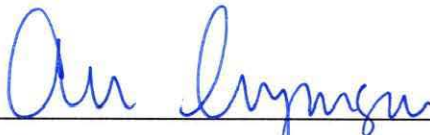
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:42
02 Std. Gas	0.081	10:43
03 Room Air	0.000	10:43
04 Std. Gas	0.081	10:44
05 Room Air	0.000	10:44
06 Std. Gas	0.081	10:45
07 Room Air	0.000	10:45

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
#4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006506  
Location = TOXL      8164.14.00 09/16  
04/08/2026      10:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:46
02 Std. Gas	0.081	10:47
03 Room Air	0.000	10:47
04 Std. Gas	0.081	10:47
05 Room Air	0.000	10:48
06 Std. Gas	0.081	10:48
07 Room Air	0.000	10:49

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
#7-9

Form 106-I8000