



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 5937 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
  - Gas Cylinder  Yes or No (If Yes, Lot # 08425080A1 Cyl. # 20)
  - Keys  Yes or No
  - Power Cord  Yes or No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: BELC
5.  Battery Check
  - Was the external battery pack replaced?  Yes or No
6.  O-Rings
  - Replaced Simulator O-Ring Yes or  No
  - Replaced Breath Tube O-Ring Yes or  No

B. General Setup and Checks:

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone:  CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).  
Display: 871 psi Regulator: 900 psi  
Display and Regulator ± 50 psi of each other  Yes or No  
Gas tank tare necessary? Yes or  No  
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

1.  Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value ≤ 0.03 AC: 0.025 AC  
Sim. Ser #: MP3063  
Lot #: 202509A  
Exp. Date: 9/10/27  
 Results ± 0.005 of known AC
2.  Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value  $\geq$  0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 2024084

Exp. Date: 8/29/26

Results  $\pm$  5% AC of known AC

3.  Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 19825080A2

Cylinder #: 20

Exp. Date: 9/5/27

4.  Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: ICS 9

Exp. Date: None

Display reads "Interferent Detect"

5.  Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6.  RFI Check (CMS Mode)

Display reads "RFI Detect"

7.  Dry Calibration Check (Level 1,C)

Test 1 0.078 Test 4 0.078 Test 7 0.078

Test 2 0.078 Test 5 0.078 Test 8 0.078

Test 3 0.077 Test 6 0.078 Test 9 0.078

Average 0.077

Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field.  Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL.

[Signature]  
Inspector Signature

07 April 2026  
Date

[Signature]  
Reviewer

08 Apr. 2026  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005937  
Location = TOXL                8164.14.00 09/16  
04/07/2026                      11:13

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup

Data Entry Mode:                Enabled  
Start Test Sequence:            DABACABA  
Display Prelim Rslt?            Yes  
Display Third Digit?            Yes  
Inhib Printer(Y/N)?            No  
Display Volume?                No  
Disable On Memfull?            Yes  
# of Print Copies?              1  
Select Std (D/W/I)?            Dry  
Standard Value?                0.080  
Standard Lot #?                 08425080A1  
Standard Cyl #?                20  
Standard Expiration?            05/05/2027  
Oper No?                        133237

Flow Cal. Date:                11/17/2017  
Slope                            606  
Intercept                       -534563

IR Calibration Date:            11/17/2017

	3um	9um
0th Coef(*100):	-30534	-23772
1st Coef(*100):	294336	142357
2nd Coef(*100):	-906	850
H2O adj(mg/l*10k):	205	250

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
ANNA INGEMANSEN

Remarks:    *Print Test*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

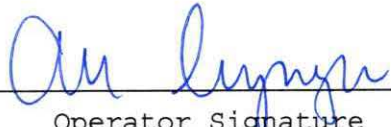
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005937  
Location = TOXL      8164.14.00 09/16  
04/07/2026      11:14

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:15
02 Std. Sol.	0.025	11:16
03 Room Air	0.000	11:16
04 Std. Sol.	0.026	11:17
05 Room Air	0.000	11:17
06 Std. Sol.	0.025	11:18
07 Room Air	0.000	11:19

08 Sim Temp = 34.0°C

Simul Ser No = MP3063  
Std Sol No = 202509A  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Low AC Check*  
*0.025AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

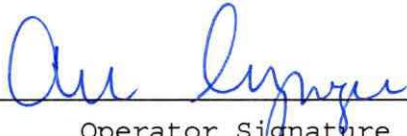
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005937  
Location = TOXL      8164.14.00 09/16  
04/07/2026      11:21

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:21
02 Std. Sol.	0.300	11:23
03 Room Air	0.000	11:23
04 Std. Sol.	0.300	11:24
05 Room Air	0.000	11:25
06 Std. Sol.	0.300	11:25
07 Room Air	0.000	11:26

08 Sim Temp = 34.0°C

Simul Ser No = MP3003  
Std Sol No = 202408H  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: High AC Check  
0.300AC

Form 106-I8000

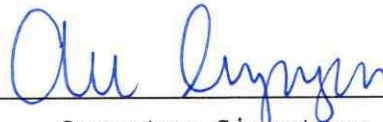
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005937  
Location = TOXL                 8164.14.00 09/16  
04/07/2026                        11:29

Test	AC	Time
01 Room Air	0.000	11:29
02 *Subject Test	INT*	11:30
03 Room Air	0.000	11:30

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                     Weight = NA  
Test = OTH                         Cit = INTERFERENT CK  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08                         Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Interferent check  
0.10AC + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005937  
Location = TOXL      8164.14.00 09/16  
04/07/2026      11:31

Test	AC	Time
01 Room Air	0.000	11:32
02 Invalid Sample	X.XXX	11:32
03 Room Air	0.000	11:33

\*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = INVALID  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08      Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Invalid sample-  
Mouth alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

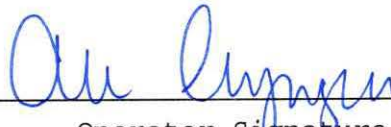
CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-005937  
Location = TOXL                              8164.14.00 09/16  
04/07/2026    11:35

Test	AC	Time
01 Diagnostic	OK	11:36
02 Room Air	0.000	11:36
03 *Subject Test	RFI*	11:37
04 Room Air	0.000	11:37

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                                      Weight = NA  
Test = OTH    Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08    Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: RFI check

Form 106-I8000

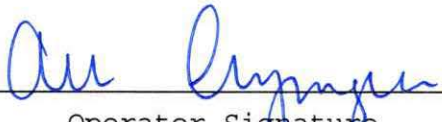
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005937  
Location = TOXL      8164.14.00 09/16  
04/07/2026      11:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:38
02 Std. Gas	0.078	11:38
03 Room Air	0.000	11:39
04 Std. Gas	0.078	11:39
05 Room Air	0.000	11:40
06 Std. Gas	0.077	11:40
07 Room Air	0.000	11:41

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry Cal check  
#1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005937  
Location = TOXL      8164.14.00 09/16  
04/07/2026      11:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:43
02 Std. Gas	0.078	11:43
03 Room Air	0.000	11:44
04 Std. Gas	0.078	11:44
05 Room Air	0.000	11:45
06 Std. Gas	0.078	11:45
07 Room Air	0.000	11:46

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
#4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005937  
Location = TOXL      8164.14.00 09/16  
04/07/2026      11:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:47
02 Std. Gas	0.078	11:47
03 Room Air	0.000	11:48
04 Std. Gas	0.078	11:48
05 Room Air	0.000	11:49
06 Std. Gas	0.078	11:49
07 Room Air	0.000	11:49

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
#7-9

Form 106-I8000