

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4939 Inspection Location: TDXL

A. Pre-Inspection

1. Items with Instrument:
  - Gas Cylinder  Yes or  No (If Yes, Lot # 08425080A1 Cyl. # 24)
  - Keys  Yes or  No
  - Power Cord  Yes or  No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: BCCC
5.  Battery Check
  - Was the external battery pack replaced? Yes or  No
6.  O-Rings
  - Replaced Simulator O-Ring  Yes or  No
  - Replaced Breath Tube O-Ring  Yes or  No

B. General Setup and Checks:

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
  - Time Zone: CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).
  - Display: 795 psi Regulator: 750 psi
  - Display and Regulator ± 50 psi of each other  Yes or  No
  - Gas tank tare necessary?  Yes or  No
  - If Yes, display readings after tare (Level 3,M,C,G):
  - Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

1.  Configure simulator for the following test (Level 1,S).
  - Wet Calibration Check - Low AC (Level 1,C)
  - Known Value ≤ 0.03 AC: 0.025 AC
  - Sim. Ser #: MP3063
  - Lot #: 202509A
  - Exp. Date: 910127
  - Results ± 0.005 of known AC
2.  Configure simulator for the following test (Level 1,S).

Post calibration adjustment

0.020AC  
MP5320  
202501E  
28Jan27

Post calibration adj.  
0.400AC  
MP3068  
202506H  
25 Jun 2027

Wet Calibration Check - High AC (Level 1,C)

Known Value  $\geq$  0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

Results  $\pm$  5% AC of known AC

3.  Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 19825080A2

Cylinder #: 20

Exp. Date: 9/5/27

4.  Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: ICS 9

Exp. Date: None

Display reads "Interferent Detect"

5.  Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6.  RFI Check (CMS Mode)

Display reads "RFI Detect"

7.  Dry Calibration Check (Level 1,C)

Test 1 0.078 Test 4 0.079 Test 7 0.079

Test 2 0.079 Test 5 0.079 Test 8 0.080

Test 3 0.079 Test 6 0.079 Test 9 0.080

Average 0.079

Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: Calibration adjustment performed due to high initial dry calibration checks.

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL.

AW Lyngse  
Inspector Signature

09 April 2026  
Date

Jesselle Putschiller  
Reviewer

10 Apr. 2026  
Date



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      11:44

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:44
02 Std. Sol.	0.026	11:45
03 Room Air	0.000	11:46
04 Std. Sol.	0.026	11:47
05 Room Air	0.000	11:47
06 Std. Sol.	0.026	11:48
07 Room Air	0.000	11:49

08 Sim Temp = 34.0°C

Simul Ser No = MP3063  
Std Sol No = 202509A  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks:

LOW AC check  
0.025AL  
Form 106-I8000

aei  
pos 4/9/26  
pre calibration  
adjustment

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      11:49

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:50
02 Std. Sol.	0.302	11:50
03 Room Air	0.000	11:51
04 Std. Sol.	0.304	11:52
05 Room Air	0.000	11:52
06 Std. Sol.	0.305	11:53
07 Room Air	0.000	11:54

08 Sim Temp = 34.0°C

Simul Ser No = MP3003  
Std Sol No = 202408H  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: High Al Check } pre calibration  
0.300AC      adjustment

Form 106-I8000

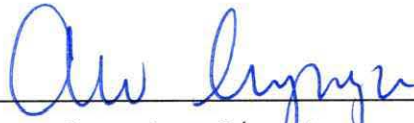
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004939  
Location = TOXL                    8164.14.00 09/16  
04/09/2026                            11:55

Test	AC	Time
01 Room Air	0.000	11:56
02 *Subject Test	INT*	11:57
03 Room Air	0.000	11:57

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                      Weight = NA  
Test = OTH                          Cit = INTERFERENT  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08                          Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Interferent check  
0.10Ac + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004939  
Location = TOXL                    8164.14.00 09/16  
04/09/2026                            12:00

Test	AC	Time
01 Room Air	0.000	12:01
02 Invalid Sample	X.XXX	12:01
03 Room Air	0.000	12:02

\*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                      Weight = NA  
Test = OTH                            Cit = INVALID  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08                          Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: Invalid Sample  
              MOUTH ALCOHOL

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

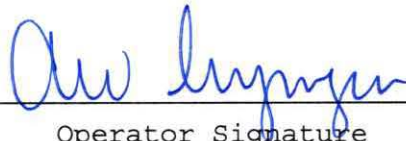
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      12:05

Test	AC	Time
01 Diagnostic	OK	12:06
02 Room Air	0.000	12:06
03 *Subject Test	RFI*	12:07
04 Room Air	0.000	12:07

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 20  
Expiration Date = 09/05/2027  
County = 08      Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
ANNA INGEMANSEN

Remarks: RFI check

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004939  
Location = TOXL                    8164.14.00 09/16  
04/09/2026                            12:08

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:09
02 Std. Gas	0.082	12:09
03 Room Air	0.000	12:10
04 Std. Gas	0.082	12:10
05 Room Air	0.000	12:11
06 Std. Gas	0.083	12:11
07 Room Air	0.000	12:11

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Dry Cal check*  
*#1-3 pre calibration*  
*adjustment*

Form 106-I8000

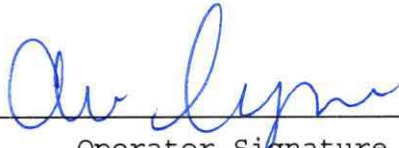
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      12:12

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:12
02 Std. Gas	0.082	12:13
03 Room Air	0.000	12:13
04 Std. Gas	0.082	12:14
05 Room Air	0.000	12:14
06 Std. Gas	0.083	12:15
07 Room Air	0.000	12:15

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
                  #4-6  
                  pre calibration adjustment  
Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      12:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:16
02 Std. Gas	0.082	12:17
03 Room Air	0.000	12:17
04 Std. Gas	0.083	12:17
05 Room Air	0.000	12:18
06 Std. Gas	0.082	12:18
07 Room Air	0.000	12:19

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
#7-9 pre cal adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      13:01

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:02
02 Std. Sol.	0.020	13:03
03 Room Air	0.000	13:04
04 Std. Sol.	0.020	13:05
05 Room Air	0.000	13:05
06 Std. Sol.	0.019	13:06
07 Room Air	0.000	13:06

08 Sim Temp = 34.0°C

Simul Ser No = MP5320  
Std Sol No = 202501E  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Low AC Check*  
*0.020Ac - post calibration*  
*adjustment.*  
Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      13:07

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:08
02 Std. Sol.	0.396	13:09
03 Room Air	0.000	13:09
04 Std. Sol.	0.400	13:10
05 Room Air	0.000	13:11
06 Std. Sol.	0.395	13:11
07 Room Air	0.000	13:12

08 Sim Temp = 34.0°C

Simul Ser No = MP3068

Std Sol No = 202506H

County = 08

Oper No. = 133237

Operator Signature  
ANNA INGEMANSEN

Remarks: High AC check

aei      0.300 -post calibration  
4/9/26      0.400 AC      adjustment.  
Form 106-I8000

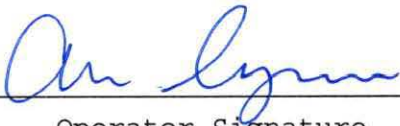
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      13:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:13
02 Std. Gas	0.078	13:14
03 Room Air	0.000	13:14
04 Std. Gas	0.079	13:14
05 Room Air	0.000	13:15
06 Std. Gas	0.079	13:15
07 Room Air	0.000	13:16

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Dry cal check #1-3*      *post calibration adjustment*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004939  
Location = TOXL                    8164.14.00 09/16  
04/09/2026                            13:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:17
02 Std. Gas	0.079	13:17
03 Room Air	0.000	13:17
04 Std. Gas	0.079	13:18
05 Room Air	0.000	13:18
06 Std. Gas	0.079	13:19
07 Room Air	0.000	13:19

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Dry cal check #4-6*                    *post calibration adjustment.*

Form 106-I8000

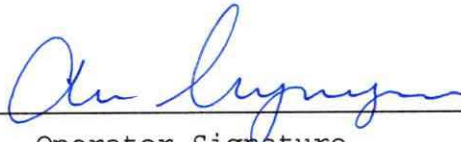
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004939  
Location = TOXL      8164.14.00 09/16  
04/09/2026      13:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:20
02 Std. Gas	0.079	13:20
03 Room Air	0.000	13:21
04 Std. Gas	0.080	13:21
05 Room Air	0.000	13:22
06 Std. Gas	0.080	13:22
07 Room Air	0.000	13:23

Lot No = 19825080A2  
Cyl No = 20  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: *dry cal check #7-9*      *post calibration adjustment.*

Form 106-I8000