



**NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION**

**INTOXILYZER® 8000 ANNUAL INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-00 5952 Inspection Location: TOXL

**A. Pre-Inspection**

1. Items with Instrument:
  - Gas Cylinder Yes or No (If Yes, Lot # 19825080A2 Cyl. # 25)
  - Keys Yes or No
  - Power Cord Yes or No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: WISH
5.  Battery Check
  - Was the external battery pack replaced? Yes or No
6.  O-Rings
  - Replaced Simulator O-Ring Yes or No
  - Replaced Breath Tube O-Ring Yes or No

**B. General Setup and Checks:**

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).  
Display: 727 psi Regulator: 750 psi  
Display and Regulator ± 50 psi of each other Yes or No  
Gas tank tare necessary? Yes or No  
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

**C. Tests (Sign and attach test records):**

1.  Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value ≤ 0.03 AC: 0.020 AC  
Sim. Ser #: MP5290  
Lot #: 202501E  
Exp. Date: 1/28/27  
 Results ± 0.005 of known AC
2.  Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value  $\geq$  0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

Results  $\pm$  5% AC of known AC

3.  Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 26-4437

Cylinder #: 104

Exp. Date: 1/29/28

4.  Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: ICS9

Exp. Date: None

Display reads "Interferent Detect"

5.  Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6.  RFI Check (CMS Mode)

Display reads "RFI Detect"

7.  Dry Calibration Check (Level 1,C)

Test 1 0.080 Test 4 0.080 Test 7 0.080

Test 2 0.080 Test 5 0.081 Test 8 0.080

Test 3 0.080 Test 6 0.080 Test 9 0.080

Average 0.080

Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: NIA

Instrument is acceptable to be used in the field.  Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL.

AW Lyman  
Inspector Signature

29 April 2026  
Date

Janelle Pitschman  
Reviewer

30 Apr. 2026  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005952  
Location = TOXL                    8164.14.00 09/16  
04/29/2026                            09:02

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-=-|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-=-|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

Current Instrument Setup

Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            19825080A2  
Standard Cyl #?            25  
Standard Expiration?        09/05/2027  
Oper No?                    133237

Flow Cal. Date:            04/16/2021  
Slope                      657  
Intercept                  -744615

IR Calibration Date:        04/16/2021  
                                  3um                            9um

-----  
0th Coef(\*100):            -24450                    -14639  
1st Coef(\*100):            266154                   132500  
2nd Coef(\*100):            2284                     1091  
H2O adj(mg/l\*10k):        516                      323

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks:            *Print Test*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005952  
Location = TOXL      8164.14.00 09/16  
04/29/2026      09:03

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 09:04 |
| 02 Std. Sol. | 0.021 | 09:04 |
| 03 Room Air  | 0.000 | 09:05 |
| 04 Std. Sol. | 0.020 | 09:06 |
| 05 Room Air  | 0.000 | 09:06 |
| 06 Std. Sol. | 0.020 | 09:07 |
| 07 Room Air  | 0.000 | 09:07 |

08 Sim Temp = 34.0°C

Simul Ser No = MP5290  
Std Sol No = 202501E  
County = 08      Oper No. = 133237

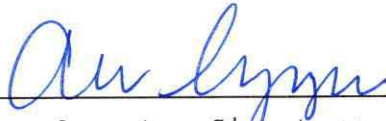

Operator Signature  
ANNA INGEMANSEN

Remarks: *Low AC Check*  
*0.020AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005952  
Location = TOXL                    8164.14.00 09/16  
04/29/2026                            09:14

WET CAL CHECK

| Test         | AC    | Time  |
|--------------|-------|-------|
| 01 Room Air  | 0.000 | 09:15 |
| 02 Std. Sol. | 0.291 | 09:16 |
| 03 Room Air  | 0.000 | 09:16 |
| 04 Std. Sol. | 0.292 | 09:17 |
| 05 Room Air  | 0.000 | 09:18 |
| 06 Std. Sol. | 0.291 | 09:18 |
| 07 Room Air  | 0.000 | 09:19 |

08 Sim Temp = 34.0°C

Simul Ser No = MP3003  
Std Sol No = 202408H  
County = 08                            Oper No. = 133237

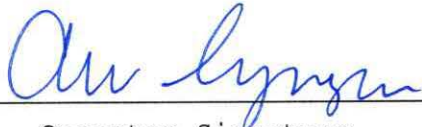

Operator Signature  
ANNA INGEMANSEN

Remarks:

High AC check  
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005952  
Location = TOXL                8164.14.00 09/16  
04/29/2026                        09:20

| Test             | AC    | Time  |
|------------------|-------|-------|
| 01 Room Air      | 0.000 | 09:21 |
| 02 *Subject Test | INT*  | 09:21 |
| 03 Room Air      | 0.000 | 09:22 |

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                    Weight = NA  
Test = OTH                        Cit = INTERFERENT  
Dr. Lic. = ND/TES989643  
Lot No = 264437  
Cyl No = 104  
Expiration Date = 01/29/2028  
County = 08                        Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Interferent check  
0.10AC + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005952  
Location = TOXL                    8164.14.00 09/16  
04/29/2026                            09:22

| Test              | AC    | Time  |
|-------------------|-------|-------|
| 01 Room Air       | 0.000 | 09:23 |
| 02 Invalid Sample | X.XXX | 09:23 |
| 03 Room Air       | 0.000 | 09:24 |

\*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                      Weight = NA  
Test = OTH                          Cit = INVALID  
Dr. Lic. = ND/TES989643  
Lot No = 264437  
Cyl No = 104  
Expiration Date = 01/29/2028  
County = 08                          Oper No. = 133237

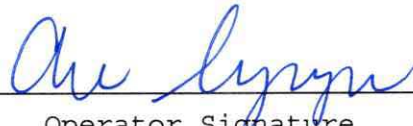

Operator Signature  
ANNA INGEMANSEN

Remarks:

Invalid sample  
mouth alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-005952  
Location = TOXL                              8164.14.00 09/16  
04/29/2026    09:25

| Test             | AC    | Time  |
|------------------|-------|-------|
| 01 Diagnostic    | OK    | 09:25 |
| 02 Room Air      | 0.000 | 09:26 |
| 03 *Subject Test | RFI*  | 09:27 |
| 04 Room Air      | 0.000 | 09:27 |

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                              Weight = NA  
Test = OTH                                      Cit = RFI  
Dr. Lic. = ND/TES989643  
Lot No = 264437  
Cyl No = 104  
Expiration Date = 01/29/2028  
County = 08                              Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
ANNA INGEMANSEN

Remarks:      *RFI check*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005952  
Location = TOXL      8164.14.00 09/16  
04/29/2026      09:27

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 09:28 |
| 02 Std. Gas | 0.080 | 09:28 |
| 03 Room Air | 0.000 | 09:29 |
| 04 Std. Gas | 0.080 | 09:29 |
| 05 Room Air | 0.000 | 09:30 |
| 06 Std. Gas | 0.080 | 09:30 |
| 07 Room Air | 0.000 | 09:31 |

Lot No = 264437  
Cyl No = 104  
Exp Date = 01/29/2028  
County = 08      Oper No. = 133237

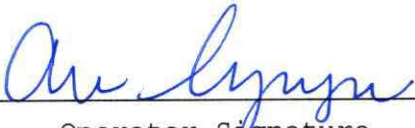  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks:      Dry cal check  
                         #1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005952  
Location = TOXL      8164.14.00 09/16  
04/29/2026      09:31

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 09:32 |
| 02 Std. Gas | 0.080 | 09:32 |
| 03 Room Air | 0.000 | 09:33 |
| 04 Std. Gas | 0.081 | 09:33 |
| 05 Room Air | 0.000 | 09:33 |
| 06 Std. Gas | 0.080 | 09:34 |
| 07 Room Air | 0.000 | 09:34 |

Lot No = 264437  
Cyl No = 104  
Exp Date = 01/29/2028  
County = 08      Oper No. = 133237

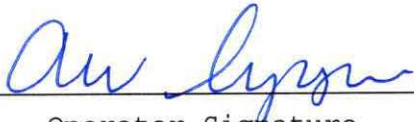  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks:      *Dry cal check*  
                      *#4-6*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005952  
Location = TOXL                    8164.14.00 09/16  
04/29/2026                            09:35

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 09:35 |
| 02 Std. Gas | 0.080 | 09:36 |
| 03 Room Air | 0.000 | 09:36 |
| 04 Std. Gas | 0.080 | 09:36 |
| 05 Room Air | 0.000 | 09:37 |
| 06 Std. Gas | 0.080 | 09:37 |
| 07 Room Air | 0.000 | 09:38 |

Lot No = 264437  
Cyl No = 104  
Exp Date = 01/29/2028  
County = 08                            Oper No. = 133237

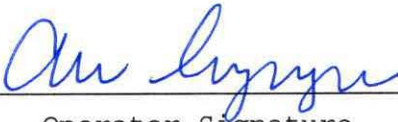  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Dry cal check  
#7-9*

Form 106-I8000