



**NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION**

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 5357 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 19825080A2 Cyl. # 20)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: GIRAF
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 956 psi Regulator: 950 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP5290
Lot #: 202501E
Exp. Date: 1/28/27
 Results ± 0.005 of known AC
2. Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value \geq 0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

Results \pm 5% AC of known AC

3. Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 25024080A3

Cylinder #: 1

Exp. Date: 10/5/26

4. Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: 1CS9

Exp. Date: None

Display reads "Interferent Detect"

5. Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6. RFI Check (CMS Mode)

Display reads "RFI Detect"

7. Dry Calibration Check (Level 1,C)

Test 1 0.081 Test 4 0.082 Test 7 0.082

Test 2 0.082 Test 5 0.082 Test 8 0.082

Test 3 0.081 Test 6 0.081 Test 9 0.082

Average 0.081

Results \pm 0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL.

[Signature]
Inspector Signature

07 May 2026
Date

[Signature]
Reviewer

07 May 2026
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 08:46

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 19825080A2
Standard Cyl #? 26
Standard Expiration? 09/05/2027
Oper No? 133237

Flow Cal. Date: 05/16/2018
Slope 573
Intercept 140460

IR Calibration Date: 06/21/2023

	3um	9um
0th Coef(*100):	-6039	-13097
1st Coef(*100):	257461	136071
2nd Coef(*100):	3187	1488
H2O adj(mg/l*10k):	315	418

***** Printer Test End *****

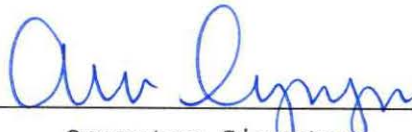

Operator Signature
ANNA INGEMANSEN

Remarks: Print Test

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 08:47

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:47
02 Std. Sol.	0.023	08:48
03 Room Air	0.000	08:49
04 Std. Sol.	0.022	08:49
05 Room Air	0.000	08:50
06 Std. Sol.	0.022	08:51
07 Room Air	0.000	08:51

08 Sim Temp = 34.0°C

Simul Ser No = MP5290
Std Sol No = 202501E
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: *LOW AC check*
0.020AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 08:53

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:54
02 Std. Sol.	0.295	08:55
03 Room Air	0.000	08:55
04 Std. Sol.	0.294	08:56
05 Room Air	0.000	08:56
06 Std. Sol.	0.295	08:57
07 Room Air	0.000	08:58

08 Sim Temp = 34.0°C

Simul Ser No = MP3003
Std Sol No = 202408H
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: High AC check
0.300AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 08:59

Test	AC	Time
01 Room Air	0.000	09:00
02 *Subject Test	INT*	09:01
03 Room Air	0.000	09:02

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 25024080A3
Cyl No = 1
Expiration Date = 10/05/2026
County = 08 Oper No. = 133237

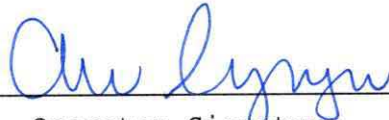

Operator Signature
ANNA INGEMANSEN

Remarks: *interferent check*
0.10AC + 0.059% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 09:02

Test	AC	Time
01 Room Air	0.000	09:03
02 Invalid Sample	X.XXX	09:04
03 Room Air	0.000	09:04

*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INVALID
Dr. Lic. = ND/TES989643
Lot No = 25024080A3
Cyl No = 1
Expiration Date = 10/05/2026
County = 08 Oper No. = 133237

Operator Signature
ANNA INGEMANSEN

Remarks: Invalid sample
Mouth Alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 09:07

Test	AC	Time
01 Diagnostic	OK	09:07
02 Room Air	0.000	09:08
03 *Subject Test	RFI*	09:08
04 Room Air	0.000	09:09

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 25024080A3
Cyl No = 1
Expiration Date = 10/05/2026
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA INGEMANSEN

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 09:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:10
02 Std. Gas	0.081	09:10
03 Room Air	0.000	09:11
04 Std. Gas	0.082	09:11
05 Room Air	0.000	09:12
06 Std. Gas	0.081	09:12
07 Room Air	0.000	09:13

Lot No = 25024080A3
Cyl No = 1
Exp Date = 10/05/2026
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Dry cal check
1-3

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 09:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:13
02 Std. Gas	0.082	09:14
03 Room Air	0.000	09:14
04 Std. Gas	0.082	09:15
05 Room Air	0.000	09:15
06 Std. Gas	0.081	09:15
07 Room Air	0.000	09:16

Lot No = 25024080A3
Cyl No = 1
Exp Date = 10/05/2026
County = 08 Oper No. = 133237

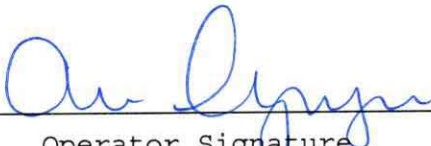

Operator Signature
ANNA INGEMANSEN

Remarks:

Dry cal check
#4-6

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005357
Location = TOXL 8164.14.00 09/16
05/07/2026 09:17

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:18
02 Std. Gas	0.082	09:18
03 Room Air	0.000	09:19
04 Std. Gas	0.082	09:19
05 Room Air	0.000	09:19
06 Std. Gas	0.082	09:20
07 Room Air	0.000	09:20

Lot No = 25024080A3
Cyl No = 1
Exp Date = 10/05/2026
County = 08 Oper No. = 133237

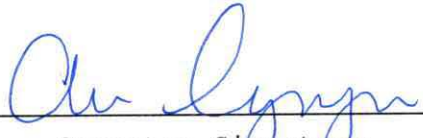

Operator Signature
ANNA INGEMANSEN

Remarks:

Dry cal check
7-9

Form 106-I8000