



**NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION**

**INTOXILYZER® 8000 ANNUAL INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-00 4944 Inspection Location: TOXL

**A. Pre-Inspection**

1. Items with Instrument:
  - Gas Cylinder Yes or No (If Yes, Lot # 25024080A3 Cyl. # 4)
  - Keys Yes or No
  - Power Cord Yes or No
2.  Download Data
3.  Upload Operator File
4.  Current Location Code: DEVL
5.  Battery Check
  - Was the external battery pack replaced? Yes or No
6.  O-Rings
  - Replaced Simulator O-Ring Yes or No
  - Replaced Breath Tube O-Ring Yes or No

**B. General Setup and Checks:**

1.  Diagnostics passed and instrument in "Ready" mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G).  
Display: 553 psi Regulator: 560 psi  
Display and Regulator ± 50 psi of each other Yes or No  
Gas tank tare necessary? Yes or No  
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

**C. Tests (Sign and attach test records):**

1.  Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value ≤ 0.03 AC: 0.020 AC  
Sim. Ser #: MP5290  
Lot #: 202501E  
Exp. Date: Has to be 1/28/27 dei 20May2026  
 Results ± 0.005 of known AC
2.  Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value  $\geq$  0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

Results  $\pm$  5% AC of known AC

3.  Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 08425080A1

Cylinder #: 23

Exp. Date: 5/5/27

4.  Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: 1CS 9

Exp. Date: None

Display reads "Interferent Detect"

5.  Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6.  RFI Check (CMS Mode)

Display reads "RFI Detect"

7.  Dry Calibration Check (Level 1,C)

Test 1 0.081 Test 4 0.081 Test 7 0.082

Test 2 0.081 Test 5 0.081 Test 8 0.082

Test 3 0.081 Test 6 0.081 Test 9 0.082

Average 0.081

Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL.

Aimee Lynne  
Inspector Signature

20 May 2026  
Date

Janella Putschner  
Reviewer

21 May 2026  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            12:19

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=-|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=-|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&\*()\_+?

Current Instrument Setup

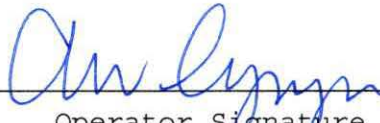
Data Entry Mode:                    Enabled  
Start Test Sequence:                DABACABA  
Display Prelim Rslt?                Yes  
Display Third Digit?                Yes  
Inhib Printer(Y/N)?                No  
Display Volume?                    No  
Disable On Memfull?                Yes  
# of Print Copies?                  1  
Select Std (D/W/I)?                Dry  
Standard Value?                    0.080  
Standard Lot #?                    25024080A3  
Standard Cyl #?                    4  
Standard Expiration?                10/05/2026  
Oper No?                            133237

Flow Cal. Date:                    07/01/2011  
Slope                                685  
Intercept                            -634740

IR Calibration Date:                07/01/2011  
    3um                                9um

-----  
0th Coef(\*100):                    -22591                                -17234  
1st Coef(\*100):                    265915                                132691  
2nd Coef(\*100):                    2841                                    1562  
H2O adj(mg/l\*10k):                559                                    425

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
ANNA INGEMANSEN

Remarks: *Print Test*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            11:44

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:44
02 Std. Sol.	0.019	11:46
03 Room Air	0.000	11:47
04 Std. Sol.	0.020	11:47
05 Room Air	0.000	11:48
06 Std. Sol.	0.020	11:49
07 Room Air	0.000	11:49

08 Sim Temp = 34.0°C

Simul Ser No = MP5290  
Std Sol No = 202501E  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks:    *LOW AC Check*  
                  *0.020AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

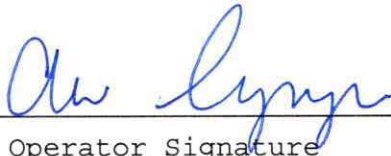
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            11:50

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:50
02 Std. Sol.	0.305	11:51
03 Room Air	0.000	11:52
04 Std. Sol.	0.306	11:53
05 Room Air	0.000	11:53
06 Std. Sol.	0.307	11:54
07 Room Air	0.000	11:54

08 Sim Temp = 34.0°C

Simul Ser No = MP3003  
Std Sol No = 202408H  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: High AC Check  
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            11:56

Test	AC	Time
01 Room Air	0.000	11:57
02 *Subject Test	INT*	11:57
03 Room Air	0.000	11:58

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                      Weight = NA  
Test = OTH                          Cit = INTERFERENT  
Dr. Lic. = ND/TES989643  
Lot No = 08425080A1  
Cyl No = 23  
Expiration Date = 05/05/2027  
County = 08                          Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: *interferent check*  
*0.10AC + 0.05% Acetone*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            12:01

Test	AC	Time
01 Room Air	0.000	12:02
02 Invalid Sample	X.XXX	12:02
03 Room Air	0.000	12:03

\*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                      Weight = NA  
Test = OTH                          Cit = INVALID  
Dr. Lic. = ND/TES989643  
Lot No = 08425080A1  
Cyl No = 23  
Expiration Date = 05/05/2027  
County = 08                          Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Invalid Sample-  
Mouth Alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            12:03

Test	AC	Time
01 Diagnostic	OK	12:04
02 Room Air	0.000	12:04
03 *Subject Test	RFI*	12:05
04 Room Air	0.000	12:05

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                            Weight = NA  
Test = OTH                                Cit = RFI  
Dr. Lic. = ND/TES989643  
Lot No = 08425080A1  
Cyl No = 23  
Expiration Date = 05/05/2027  
County = 08                                Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
ANNA INGEMANSEN

Remarks:

RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            12:06

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:06
02 Std. Gas	0.081	12:07
03 Room Air	0.000	12:07
04 Std. Gas	0.081	12:07
05 Room Air	0.000	12:08
06 Std. Gas	0.081	12:08
07 Room Air	0.000	12:09

Lot No = 08425080A1  
Cyl No = 23  
Exp Date = 05/05/2027  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Dry cal check  
#1-3*

Form 106-I8000

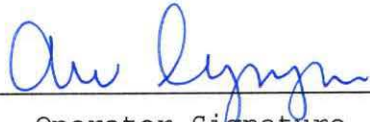
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004944  
Location = TOXL                    8164.14.00 09/16  
05/20/2026                            12:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:10
02 Std. Gas	0.081	12:10
03 Room Air	0.000	12:11
04 Std. Gas	0.081	12:11
05 Room Air	0.000	12:11
06 Std. Gas	0.081	12:12
07 Room Air	0.000	12:12

Lot No = 08425080A1  
Cyl No = 23  
Exp Date = 05/05/2027  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *Dry cal check*  
*#4-6*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004944  
Location = TOXL      8164.14.00 09/16  
05/20/2026      12:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:14
02 Std. Gas	0.082	12:14
03 Room Air	0.000	12:14
04 Std. Gas	0.082	12:15
05 Room Air	0.000	12:15
06 Std. Gas	0.082	12:16
07 Room Air	0.000	12:16

Lot No = 08425080A1  
Cyl No = 23  
Exp Date = 05/05/2027  
County = 08      Oper No. = 133237

  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
#7-9

Form 106-I8000