



**NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION**

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 60089 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
 - Gas Cylinder Yes or No (If Yes, Lot # 08425080A1 Cyl. # 23)
 - Keys Yes or No
 - Power Cord Yes or No
2. Download Data
3. Upload Operator File
4. Current Location Code: DKPD
5. Battery Check
 - Was the external battery pack replaced? Yes or No
6. O-Rings
 - Replaced Simulator O-Ring Yes or No
 - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. Diagnostics passed and instrument in "Ready" mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G).
Display: 412 psi Regulator: 450 psi
Display and Regulator ± 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value ≤ 0.03 AC: 0.025 AC
Sim. Ser #: MP30103
Lot #: 202509A
Exp. Date: 9/10/27
 Results ± 0.005 of known AC
2. Configure simulator for the following test (Level 1,S).

*post calibration
adjustment - 0.020 AC
MP5290
202501E
1/28/27*

Wet Calibration Check - High AC (Level 1,C)

Known Value \geq 0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

Results \pm 5% AC of known AC

3. Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 19825080A2

Cylinder #: 20

Exp. Date: 9/5/27

4. Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: ICS 9

Exp. Date: None

Display reads "Interferent Detect"

5. Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6. RFI Check (CMS Mode)

Display reads "RFI Detect"

7. Dry Calibration Check (Level 1,C)

Test 1 0.077 Test 4 0.077 Test 7 0.076

Test 2 0.077 Test 5 0.076 Test 8 0.077

Test 3 0.077 Test 6 0.076 Test 9 0.077

Average 0.076

Results \pm 0.005 AC of known AC

post calibration adjustment
0.400AC
MP3065
202506H
25 June 27

post calibration adjustment
0.080AC
25024080A3
01
10/05/2026

D. Remarks/Maintenance: NIAaei 5/15/26 Due to lower dry calibration values, a calibration adjustment was performed. Post calibration adjustment dry cal values are: 0.080, 0.081, 0.081, 0.080, 0.080, 0.080, 0.080, 0.080, 0.080 for an average of 0.080.

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. Instrument was swapped, so changed to TOXL

Chris Lynne
Inspector Signature

15 May 2026
Date
~~08 April 2026~~ aei 5/15/26

Janette Purtschmer
Reviewer

18 May 2026
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
04/08/2026 11:01

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ &* () _ + ?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ &* () _ + ?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer (Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 08425080A1
Standard Cyl #? 23
Standard Expiration? 05/05/2027
Oper No? 133237

Flow Cal. Date: 05/29/2020
Slope 643
Intercept -576193

IR Calibration Date: 05/29/2020
 3um 9um

0th Coef (*100): -25870 -28277
1st Coef (*100): 287704 139899
2nd Coef (*100): 26 744
H2O adj (mg/l*10k): 293 328

***** Printer Test End *****



Operator Signature
ANNA INGEMANSEN

Remarks: *pnnt Test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
04/08/2026 11:12

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:12
02 Std. Sol.	0.297	11:13
03 Room Air	0.000	11:14
04 Std. Sol.	0.298	11:14
05 Room Air	0.000	11:15
06 Std. Sol.	0.297	11:16
07 Room Air	0.000	11:16

08 Sim Temp = 34.0°C

Simul Ser No = MP3003
Std Sol No = 202408H
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: High AC check pre calibration
 0.300 AC adjustment

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
04/08/2026 11:17

Test	AC	Time
01 Room Air	0.000	11:18
02 *Subject Test	INT*	11:18
03 Room Air	0.000	11:19

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT CK
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 20
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: Interferent Check
0.10AC + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
04/08/2026 11:19

Test	AC	Time
01 Room Air	0.000	11:20
02 Invalid Sample	X.XXX	11:21
03 Room Air	0.000	11:22

*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INVALID
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 20
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: *Invalid sample
mouth alcohol*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
04/08/2026 11:22

Test	AC	Time
01 Diagnostic	OK	11:23
02 Room Air	0.000	11:24
03 *Subject Test	RFI*	11:24
04 Room Air	0.000	11:25

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 20
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ANNA INGEMANSEN

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
04/08/2026 11:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:29
02 Std. Gas	0.077	11:29
03 Room Air	0.000	11:30
04 Std. Gas	0.076	11:30
05 Room Air	0.000	11:31
06 Std. Gas	0.076	11:31
07 Room Air	0.000	11:31

Lot No = 19825080A2
Cyl No = 20
Exp Date = 09/05/2027
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: *Dry Cal check #4-6* *pre calibration adjustment*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
04/08/2026 11:35

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:36
02 Std. Gas	0.076	11:36
03 Room Air	0.000	11:37
04 Std. Gas	0.077	11:37
05 Room Air	0.000	11:37
06 Std. Gas	0.077	11:38
07 Room Air	0.000	11:38

Lot No = 19825080A2
Cyl No = 20
Exp Date = 09/05/2027
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check #7-9 pre calibration adjustment

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
05/15/2026 12:32

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:33
02 Std. Sol.	0.021	12:35
03 Room Air	0.000	12:35
04 Std. Sol.	0.021	12:36
05 Room Air	0.000	12:36
06 Std. Sol.	0.021	12:37
07 Room Air	0.000	12:38

08 Sim Temp = 34.0°C

Simul Ser No = MP5290
Std Sol No = 202501E
County = 08 Oper No. = 133237

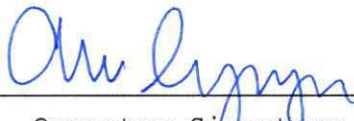

Operator Signature
ANNA INGEMANSEN

Remarks: *LOW AC check* *post calibration*
 0.020 AC *adjustment.*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
05/15/2026 12:40

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:41
02 Std. Sol.	0.401	12:42
03 Room Air	0.000	12:42
04 Std. Sol.	0.402	12:43
05 Room Air	0.000	12:43
06 Std. Sol.	0.401	12:44
07 Room Air	0.000	12:45

08 Sim Temp = 34.0°C

Simul Ser No = MP3065
Std Sol No = 202506H
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks:

High AC Check post calibration
0.400AC adjustment.

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = TOXL 8164.14.00 09/16
05/15/2026 12:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:48
02 Std. Gas	0.080	12:49
03 Room Air	0.000	12:49
04 Std. Gas	0.081	12:50
05 Room Air	0.000	12:50
06 Std. Gas	0.081	12:51
07 Room Air	0.000	12:51

Lot No = 25024080A3
Cyl No = 1
Exp Date = 10/05/2026
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check #1-3 post calibration adjustment.

Form 106-I8000

