



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4947 Inspection Location: TOXL

A. Pre-Inspection

- Items with Instrument:
  - Gas Cylinder Yes or No (If Yes, Lot # \_\_\_\_\_ Cyl. # \_\_\_\_\_)
  - Keys Yes or No
  - Power Cord Yes or No
- Download Data
- Upload Operator File
- Current Location Code: TOXL
- Battery Check
  - Was the external battery pack replaced? Yes or No
- O-Rings
  - Replaced Simulator O-Ring Yes or No
  - Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

- Diagnostics passed and instrument in "Ready" mode
- Breath tube heated
- Date, time and location code (Level 2,E). Re-set if necessary.  
Time Zone: CST or MDT (Time on test records will be in time zone circled).
- Print test (Level 1,P). Sign and attach test record.
- Tank monitor (Level 3,D,G).  
Display: 778 psi Regulator: 775 <sup>at 5/28/26</sup> 750 psi  
Display and Regulator ± 50 psi of each other Yes or No  
Gas tank tare necessary? Yes or No  
If Yes, display readings after tare (Level 3,M,C,G):  
Display: \_\_\_\_\_ psi Regulator: \_\_\_\_\_ psi

C. Tests (Sign and attach test records):

- Configure simulator for the following test (Level 1,S).  
Wet Calibration Check - Low AC (Level 1,C)  
Known Value ≤ 0.03 AC: 0.020 AC  
Sim. Ser #: MP5290  
Lot #: 202501E  
Exp. Date: 1/29/27  
 Results ± 0.005 of known AC
- Configure simulator for the following test (Level 1,S).

Wet Calibration Check - High AC (Level 1,C)

Known Value  $\geq$  0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

Results  $\pm$  5% AC of known AC

3.  Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 19825080A2

Cylinder #: 23

Exp. Date: 9/5/27

4.  Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: 1CS9

Exp. Date: None

Display reads "Interferent Detect"

5.  Invalid Sample (Level 1,B)

Display reads "Invalid Sample"

6.  RFI Check (CMS Mode)

Display reads "RFI Detect"

7.  Dry Calibration Check (Level 1,C)

Test 1 0.077 Test 4 0.078 Test 7 0.078

Test 2 0.077 Test 5 0.078 Test 8 0.078

Test 3 0.078 Test 6 0.078 Test 9 0.078

Average 0.077

Results  $\pm$  0.005 AC of known AC

D. Remarks/Maintenance: N/A

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: \_\_\_\_\_

If Yes, change location code back to A.4 unless A.4 is TOXL.

*Aur Lyman*  
Inspector Signature

28 May 2026  
Date

*Jessika Putschler*  
Reviewer

29 May 2026  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004947  
Location = TOXL                    8164.14.00 09/16  
05/28/2026                            09:58

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-=  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-=  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

Current Instrument Setup

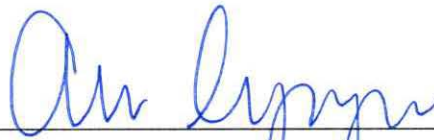
Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            264437  
Standard Cyl #?            114  
Standard Expiration?       01/29/2028  
Oper No?                    133237

Flow Cal. Date:            04/07/2020  
Slope                      618  
Intercept                  -565524

IR Calibration Date:        04/09/2024  
                                  3um                    9um

-----  
0th Coef(\*100):            -21002                    -23184  
1st Coef(\*100):            264237                    133599  
2nd Coef(\*100):            1927                      1247  
H2O adj(mg/l\*10k):        409                        438

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
ANNA INGEMANSEN

Remarks: *print Test*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

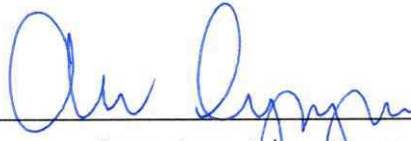
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004947  
Location = TOXL                    8164.14.00 09/16  
05/28/2026                            09:59

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:59
02 Std. Sol.	0.020	10:00
03 Room Air	0.000	10:01
04 Std. Sol.	0.020	10:02
05 Room Air	0.000	10:02
06 Std. Sol.	0.020	10:03
07 Room Air	0.000	10:03

08 Sim Temp = 34.0°C

Simul Ser No = MP5290  
Std Sol No = 202501E  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: *LOW AC Check*  
*0.020AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

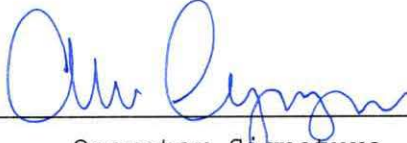
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004947  
Location = TOXL      8164.14.00 09/16  
05/28/2026      10:05

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:05
02 Std. Sol.	0.296	10:06
03 Room Air	0.000	10:07
04 Std. Sol.	0.298	10:07
05 Room Air	0.000	10:08
06 Std. Sol.	0.296	10:09
07 Room Air	0.000	10:09

08 Sim Temp = 34.0°C

Simul Ser No = MP3003  
Std Sol No = 202408H  
County = 08      Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: High AC Check  
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004947  
Location = TOXL      8164.14.00 09/16  
05/28/2026      10:11

Test	AC	Time
01 Room Air	0.000	10:12
02 *Subject Test	INT*	10:12
03 Room Air	0.000	10:13

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = OTH      Cit = INTERFERENT  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 23  
Expiration Date = 09/05/2027  
County = 08      Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Interferent check  
0.10AL + 0.05% Acetone

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004947  
Location = TOXL                 8164.14.00 09/16  
05/28/2026                        10:14

Test	AC	Time
01 Room Air	0.000	10:14
02 Invalid Sample	X.XXX	10:15
03 Room Air	0.000	10:15

\*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                    Weight = NA  
Test = OTH                        Cit = INVALID  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 23  
Expiration Date = 09/05/2027  
County = 08                        Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks: Invalid sample  
Mouth alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

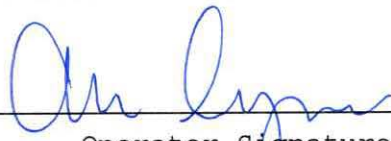
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004947  
Location = TOXL                    8164.14.00 09/16  
05/28/2026                            10:16

Test	AC	Time
01 Diagnostic	OK	10:17
02 Room Air	0.000	10:18
03 *Subject Test	RFI*	10:19
04 Room Air	0.000	10:19

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                      Weight = NA  
Test = OTH                            Cit = RFI  
Dr. Lic. = ND/TES989643  
Lot No = 19825080A2  
Cyl No = 23  
Expiration Date = 09/05/2027  
County = 08                          Oper No. = 133237

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: RFI Check

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004947  
Location = TOXL                    8164.14.00 09/16  
05/28/2026                            10:20

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:21
02 Std. Gas	0.077	10:21
03 Room Air	0.000	10:22
04 Std. Gas	0.077	10:22
05 Room Air	0.000	10:22
06 Std. Gas	0.078	10:23
07 Room Air	0.000	10:23

Lot No = 19825080A2  
Cyl No = 23  
Exp Date = 09/05/2027  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks:    Dry cal check  
                  #1-3  
                  Form 106-I8000

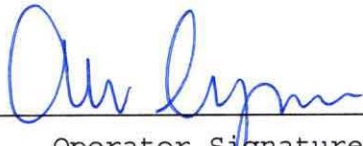
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004947  
Location = TOXL                    8164.14.00 09/16  
05/28/2026                            10:24

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:24
02 Std. Gas	0.078	10:25
03 Room Air	0.000	10:25
04 Std. Gas	0.078	10:25
05 Room Air	0.000	10:26
06 Std. Gas	0.078	10:26
07 Room Air	0.000	10:27

Lot No = 19825080A2  
Cyl No = 23  
Exp Date = 09/05/2027  
County = 08                            Oper No. = 133237

  
\_\_\_\_\_  
Operator Signature  
ANNA INGEMANSEN

Remarks: Dry cal check  
              #4-6

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004947  
Location = TOXL      8164.14.00 09/16  
05/28/2026      10:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:28
02 Std. Gas	0.078	10:28
03 Room Air	0.000	10:29
04 Std. Gas	0.078	10:29
05 Room Air	0.000	10:29
06 Std. Gas	0.078	10:30
07 Room Air	0.000	10:30

Lot No = 19825080A2  
Cyl No = 23  
Exp Date = 09/05/2027  
County = 08      Oper No. = 133237



Operator Signature  
ANNA INGEMANSEN

Remarks:

Dry cal check  
#7-9

Form 106-I8000