



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59281 (06/2018)

Serial Number 80-004954	Instrument Location Cass County Jail-Booking
Reason for Install/Repair	
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): **No maint Required/Performed!**
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature Kathryn M. Allen #3671 CC80	Date 5-28-2026
---	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By Anna Ingemansen	Ann Ingemansen	Certified Date 03 June 2026
---	-----------------------	---------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004954
Location = CASS 8164.14.00 09/16
05/28/2026 18:25

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

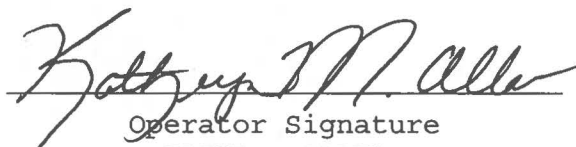
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 19825080A2
Standard Cyl #? 35
Standard Expiration? 09/05/2027
Oper No? 090801

Flow Cal. Date: 08/27/2012
Slope 670
Intercept -570610

IR Calibration Date: 04/02/2024
 3um 9um

0th Coef(*100): -20499 -21878
1st Coef(*100): 255404 129613
2nd Coef(*100): 1977 1285
H2O adj(mg/l*10k): 414 417

***** Printer Test End *****


Operator Signature
KATHRYN ALLEN

Remarks:

Print test OK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004954
Location = CASS 8164.14.00 09/16
05/28/2026 18:31

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:32
02 Std. Gas	0.077	18:32
03 Room Air	0.000	18:33
04 Std. Gas	0.078	18:33
05 Room Air	0.000	18:34
06 Std. Gas	0.079	18:34
07 Room Air	0.000	18:35

Lot No = 19825080A2
Cyl No = 35
Exp Date = 09/05/2027
County = 09 Oper No. = 090801

Kathryn M. Allen (18) #3671
Operator Signature
KATHRYN ALLEN

Remarks: Dry CAL Results w/in normal
Range !!
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004954
Location = CASS 8164.14.00 09/16
05/28/2026 18:38

Test	AC	Time
01 Room Air	0.000	18:39
02 Reference	RFI*	18:39
03 Room Air	0.000	18:40

*Invalid Test
Inhibited - RFI

Sub Name = RFI TEST, TEST TEST
Sub DOB = 01/01/1900
Sub Sex = Female Weight = 200
Test = DUI Cit = RFI TEST
Dr. Lic. = ND/NA
Lot No = 19825080A2
Cyl No = 35
Expiration Date = 09/05/2027
County = 09 Oper No. = 090801

Kathryn M. Allen #31071 CC80
Operator Signature
KATHRYN ALLEN

Remarks: RFI testing - Good !!
U

Form 106-I8000