



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 90-004204	Instrument Location ROLCA (ROLETTE COUNTY SO.)
Reason for Install/Repair	
<input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) ANNUAL INSPECTION AT CRIME LABORATORY	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): NA
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date 5/29/26
-------------------------------	------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By Anna Ingemansen	Certified Date 04 June 2026
---	---------------------------------------

For clarification, this installation was performed at Rolette County SO, after the annual inspection at the Crime Laboratory. 04June2026 AEI

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004204
Location = ROLL 8164.14.00 09/16
05/29/2026 17:06

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup

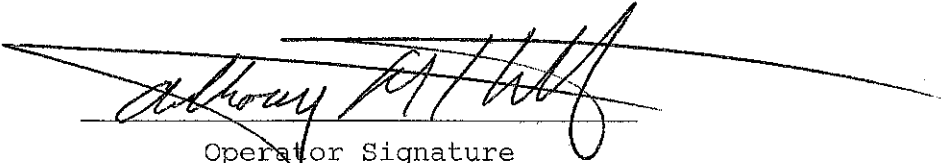
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 25024080A3
Standard Cyl #? 51
Standard Expiration? 10/05/2026
Oper No? 133866

Flow Cal. Date: 04/15/2020
Slope 657
Intercept -673032

IR Calibration Date: 06/22/2023
 3um 9um

	3um	9um
0th Coef(*100):	-20901	-22715
1st Coef(*100):	264345	135832
2nd Coef(*100):	2957	1309
H2O adj(mg/l*10k):	448	454

***** Printer Test End *****


Operator Signature
ANTHONY HILL

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004204
Location = ROLL 8164.14.00 09/16
05/29/2026 17:07

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	17:07
02 Std. Gas	0.082	17:08
03 Room Air	0.000	17:08
04 Std. Gas	0.080	17:09
05 Room Air	0.000	17:09
06 Std. Gas	0.081	17:09
07 Room Air	0.000	17:10

Lot No = 25024080A3
Cyl No = 51
Exp Date = 10/05/2026
County = 40 Oper No. = 133866


Operator Signature
ANTHONY HILL

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004204
Location = ROLL 8164.14.00 09/16
05/29/2026 17:11

Test	AC	Time
01 Room Air	0.000	17:14
02 Reference	RFI*	17:15
03 Room Air	RFI*	17:15

*Invalid Test
Inhibited - RFI

Sub Name = TEST, TEST TEST
Sub DOB = 05/29/2000
Sub Sex = Male Weight = 150
Test = OTH Cit = NA
Dr. Lic. = ND/NA
Lot No = 25024080A3
Cyl No = 51
Expiration Date = 10/05/2026
County = 40 Oper No. = 133866


Operator Signature
ANTHONY HILL

Remarks:

Form 106-I8000