



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 4950

Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # 08425080A1 Cyl. # 13)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: MOHL
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 736 psi Regulator: 750 psi
Display and Regulator $\pm$ 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value $\leq$ 0.03 AC: 0.020 AC
Sim. Ser #: MP5290
Lot #: 202501E
Exp. Date: 1/28/27
☒ Results $\pm$ 0.005 of known AC
2. ☒ Configure simulator for the following test (Level 1,S).

Post calibration adjust.

0.025AC
MP 5317
202509A
9/10/27

Wet Calibration Check - High AC (Level 1,C)

Known Value $\geq$ 0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

☒ Results $\pm$ 5% AC of known AC

Post calibration adjust.

0.400

MP3065

202506H

25 June 2027

3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 264437

Cylinder #: 104

Exp. Date: 1/29/28

4. ☒ Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: 1CS9

Exp. Date: None

☒ Display reads "Interferent Detect"

5. ☒ Invalid Sample (Level 1,B)

☒ Display reads "Invalid Sample"

6. ☒ RFI Check (CMS Mode)

☒ Display reads "RFI Detect"

7. ☒ Dry Calibration Check (Level 1,C) - post calibration adjustment.

Test 1 0.080 Test 4 0.079 Test 7 0.079

Test 2 0.079 Test 5 0.079 Test 8 0.079

Test 3 0.079 Test 6 0.079 Test 9 0.080

Average 0.079

☒ Results $\pm$ 0.005 AC of known AC

D. Remarks/Maintenance: a calibration adjustment was performed due to the low AC values of (0.077, 0.077, 0.077, 0.077, 0.077 and 0.077) during the dry calibration check.

Instrument is acceptable to be used in the field. ☒ Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☐ N/A. Instrument was swapped.

[Signature]

Inspector Signature

10 June 2026

Date

[Signature]

Reviewer

16 June 2026

Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:12

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 08425080A1
Standard Cyl #? 13
Standard Expiration? 05/05/2027
Oper No? 133237

Flow Cal. Date: 01/18/2010
Slope 774
Intercept -908904

IR Calibration Date: 04/19/2024

	3um	9um
0th Coef(*100):	-28189	-35353
1st Coef(*100):	278200	142117
2nd Coef(*100):	2249	1342
H2O adj(mg/l*10k):	369	463

***** Printer Test End *****


Operator Signature
ANNA INGEMANSEN

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:13

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:14
02 Std. Sol.	0.017	12:14
03 Room Air	0.000	12:15
04 Std. Sol.	0.017	12:16
05 Room Air	0.000	12:16
06 Std. Sol.	0.017	12:17
07 Room Air	0.000	12:17

08 Sim Temp = 34.0°C

Simul Ser No = MP5290
Std Sol No = 202501E
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Low AC Check
0.020

pre calibration
adjustment

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:18

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:19
02 Std. Sol.	0.291	12:20
03 Room Air	0.000	12:20
04 Std. Sol.	0.292	12:21
05 Room Air	0.000	12:22
06 Std. Sol.	0.293	12:22
07 Room Air	0.000	12:23

08 Sim Temp = 34.0°C

Simul Ser No = MP3003
Std Sol No = 202408H
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: High AC Check pre calibration
0.300A adjustment

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:24

Test	AC	Time
01 Room Air	0.000	12:25
02 *Subject Test	INT*	12:25
03 Room Air	0.000	12:26

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 264437
Cyl No = 104
Expiration Date = 01/29/2028
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Interferent check
0.10AC + 0.05% Acetone
Form 106-I8000

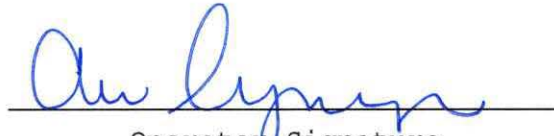
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:26

Test	AC	Time
01 Room Air	0.000	12:27
02 Invalid Sample	X.XXX	12:27
03 Room Air	0.000	12:28

*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INVALID
Dr. Lic. = ND/TES989643
Lot No = 264437
Cyl No = 104
Expiration Date = 01/29/2028
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: Invalid Sample
mouth alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

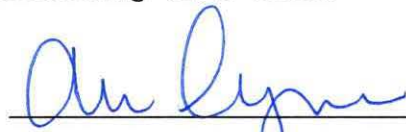
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:28

Test	AC	Time
01 Diagnostic	OK	12:29
02 Room Air	0.000	12:30
03 *Subject Test	RFI*	12:30
04 Room Air	0.000	12:30

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI
Dr. Lic. = ND/TES989643
Lot No = 264437
Cyl No = 104
Expiration Date = 01/29/2028
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA INGEMANSEN

Remarks:

RFI Check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:31

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:31
02 Std. Gas	0.077	12:32
03 Room Air	0.000	12:32
04 Std. Gas	0.077	12:32
05 Room Air	0.000	12:33
06 Std. Gas	0.077	12:33
07 Room Air	0.000	12:34

Lot No = 264437
Cyl No = 104
Exp Date = 01/29/2028
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check #1-3
pre cal. adjustment
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/05/2026 12:34

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:35
02 Std. Gas	0.077	12:35
03 Room Air	0.000	12:35
04 Std. Gas	0.077	12:36
05 Room Air	0.000	12:36
06 Std. Gas	0.077	12:37
07 Room Air	0.000	12:37

Lot No = 264437
Cyl No = 104
Exp Date = 01/29/2028
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check #4-6
pre calibration adjustment
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/10/2026 13:55

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:55
02 Std. Sol.	0.023	13:57
03 Room Air	0.000	13:57
04 Std. Sol.	0.023	13:58
05 Room Air	0.000	13:59
06 Std. Sol.	0.023	13:59
07 Room Air	0.000	14:00

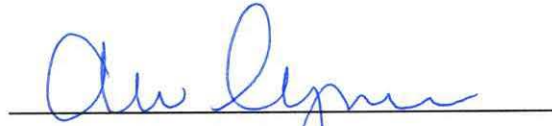
08 Sim Temp = 34.0°C

Simul Ser No = MP5317

Std Sol No = 202509A

County = 08

Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks:

Low AC Check Post calibration
0.025AC adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/10/2026 14:08

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:09
02 Std. Sol.	0.393	14:09
03 Room Air	0.000	14:10
04 Std. Sol.	0.393	14:11
05 Room Air	0.000	14:11
06 Std. Sol.	0.392	14:12
07 Room Air	0.000	14:13

08 Sim Temp = 34.0°C

Simul Ser No = MP3065
Std Sol No = 202506H
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: ~~High AC~~ ^{AEI} 6/10/26 ~~cal check~~
High AC check 0.400 AC post calibration
adjustment.
Form 106-I8000

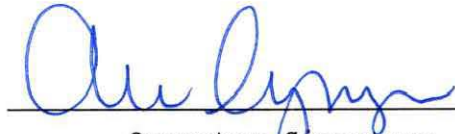
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/10/2026 14:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:17
02 Std. Gas	0.080	14:17
03 Room Air	0.000	14:18
04 Std. Gas	0.079	14:18
05 Room Air	0.000	14:19
06 Std. Gas	0.079	14:19
07 Room Air	0.000	14:20

Lot No = 264437
Cyl No = 104
Exp Date = 01/29/2028
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check Post calibration
 #1-3 adjustment
Form 106-I8000

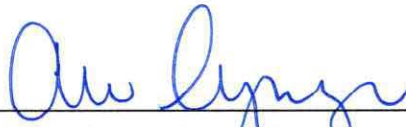
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/10/2026 14:20

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:21
02 Std. Gas	0.079	14:21
03 Room Air	0.000	14:22
04 Std. Gas	0.079	14:22
05 Room Air	0.000	14:23
06 Std. Gas	0.079	14:23
07 Room Air	0.000	14:24

Lot No = 264437
Cyl No = 104
Exp Date = 01/29/2028
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks:

Dry cal check
#4-6

post calibration
adjustment.

Form 106-I8000

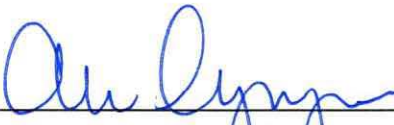
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = TOXL 8164.14.00 09/16
06/10/2026 14:24

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:24
02 Std. Gas	0.079	14:25
03 Room Air	0.000	14:25
04 Std. Gas	0.079	14:26
05 Room Air	0.000	14:26
06 Std. Gas	0.080	14:27
07 Room Air	0.000	14:27

Lot No = 264437
Cyl No = 104
Exp Date = 01/29/2028
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks: Dry cal check post calibration
 #7-q adjustment.

Form 106-I8000