



NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION

INTOXILYZER® 8000 ANNUAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-00 3065 Inspection Location: TOXL

A. Pre-Inspection

1. Items with Instrument:
Gas Cylinder Yes or No (If Yes, Lot # _____ Cyl. # _____)
Keys Yes or No
Power Cord Yes or No
2. ☒ Download Data
3. ☒ Upload Operator File
4. ☒ Current Location Code: TOXL
5. ☒ Battery Check
Was the external battery pack replaced? Yes or No
6. ☒ O-Rings
Replaced Simulator O-Ring Yes or No
Replaced Breath Tube O-Ring Yes or No

B. General Setup and Checks:

1. ☒ Diagnostics passed and instrument in "Ready" mode
2. ☒ Breath tube heated
3. ☒ Date, time and location code (Level 2,E). Re-set if necessary.
Time Zone: CST or MDT (Time on test records will be in time zone circled).
4. ☒ Print test (Level 1,P). Sign and attach test record.
5. ☒ Tank monitor (Level 3,D,G).
Display: 273 psi Regulator: 275 psi
Display and Regulator $\pm$ 50 psi of each other Yes or No
Gas tank tare necessary? Yes or No
If Yes, display readings after tare (Level 3,M,C,G):
Display: _____ psi Regulator: _____ psi

C. Tests (Sign and attach test records):

1. ☒ Configure simulator for the following test (Level 1,S).
Wet Calibration Check - Low AC (Level 1,C)
Known Value $\leq$ 0.03 AC: 0.020 AC
Sim. Ser #: MP5290
Lot #: 202501E
Exp. Date: 1/25/27
☒ Results $\pm$ 0.005 of known AC
2. ☒ Configure simulator for the following test (Level 1,S).

Post calibration
adjustment
0.025Ac
MP5317
202509A
9/10/27

Wet Calibration Check - High AC (Level 1,C)

Known Value $\geq$ 0.25 AC: 0.300 AC

Sim. Ser #: MP3003

Lot #: 202408H

Exp. Date: 8/29/26

☒ Results $\pm$ 5% AC of known AC

3. ☒ Configure dry gas standard for the remaining tests (Level 1,S).

Known Value : 0.080 AC

Gas Cylinder Lot #: 19825080A2

Cylinder #: 23

Exp. Date: 9/5/27

4. ☒ Interferent Check (Level 1,B)

Known Value: 0.10 AC + 0.05% Acetone

Sim. Ser #: DR7352

Lot #: 1CS9

Exp. Date: None

☒ Display reads "Interferent Detect"

5. ☒ Invalid Sample (Level 1,B)

☒ Display reads "Invalid Sample"

6. ☒ RFI Check (CMS Mode)

☒ Display reads "RFI Detect"

7. ☒ Dry Calibration Check (Level 1,C)

Test 1 0.079

Test 4 0.079

Test 7 0.079

Test 2 0.079

Test 5 0.079

Test 8 0.080

Test 3 0.079

Test 6 0.080

Test 9 0.080

Average 0.079

☒ Results $\pm$ 0.005 AC of known AC

post calibration adjustment.

0.400 AC
MP3065
202506H
25 June 27

Post calibration adjustment

0.080 AC
26-4437
114
1/29/28

D. Remarks/Maintenance: Calibration Adjustment values was performed due to values of 0.078, 0.077, 0.077, 0.077, 0.077 and 0.077. The values listed above at 7., are post calibration adjustment.

Instrument is acceptable to be used in the field. Yes or No

If No, state reason(s) why: _____

If Yes, change location code back to A.4 unless A.4 is TOXL. ☒

Ann Lyman
Inspector Signature

25 June 2026
Date

Janelle Putschner
Reviewer

29 June 2026
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:16

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 14323080A4
Standard Cyl #? 17
Standard Expiration? 06/05/2025
Oper No? 133237

Flow Cal. Date: 05/19/2017
Slope 612
Intercept 21223

IR Calibration Date: 08/23/2016
3um 9um

0th Coef(*100):	-14934	-12309
1st Coef(*100):	289519	141483
2nd Coef(*100):	1834	736
H2O adj(mg/l*10k):	268	136

***** Printer Test End *****



Operator Signature
ANNA INGEMANSEN

Remarks: Print Test

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:16

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:17
02 Std. Sol.	0.022	14:18
03 Room Air	0.000	14:19
04 Std. Sol.	0.021	14:19
05 Room Air	0.000	14:20
06 Std. Sol.	0.021	14:21
07 Room Air	0.000	14:21

08 Sim Temp = 34.0°C

Simul Ser No = MP5290

Std Sol No = 202501E

County = 08

Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Low AC Check
0.020AC

pre calibration
adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:22

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:22
02 Std. Sol.	0.298	14:23
03 Room Air	0.000	14:24
04 Std. Sol.	0.297	14:25
05 Room Air	0.000	14:25
06 Std. Sol.	0.297	14:26
07 Room Air	0.000	14:26


08 Sim Temp = 34.0°C

Simul Ser No = MP3003

Std Sol No = 202408H

County = 08

Oper No. = 133237

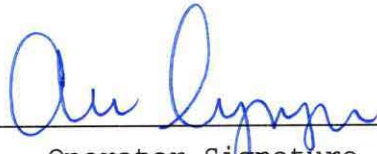

Operator Signature
ANNA INGEMANSEN

Remarks: High AC check pre calibration
 0.300AC adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:33

Test	AC	Time
01 Room Air	0.000	14:34
02 *Subject Test	INT*	14:35
03 Room Air	0.000	14:35

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 23
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks: Interferent check
0.10Ac + 0.05% Acetone

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:36

Test	AC	Time
01 Room Air	0.000	14:36
02 Invalid Sample	X.XXX	14:37
03 Room Air	0.000	14:37

*Invalid Test - Mouth Alcohol

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = INVALID
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 23
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Invalid Sample
Mouth Alcohol

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:38

Test	AC	Time
01 Diagnostic	OK	14:38
02 Room Air	0.000	14:39
03 *Subject Test	RFI*	14:39
04 Room Air	0.000	14:40

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = OTH Cit = RFI
Dr. Lic. = ND/TES989643
Lot No = 19825080A2
Cyl No = 23
Expiration Date = 09/05/2027
County = 08 Oper No. = 133237

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
ANNA INGEMANSEN

Remarks: RFI Check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:40

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:41
02 Std. Gas	0.078	14:41
03 Room Air	0.000	14:42
04 Std. Gas	0.077	14:42
05 Room Air	0.000	14:42
06 Std. Gas	0.077	14:43
07 Room Air	0.000	14:43

Lot No = 19825080A2
Cyl No = 23
Exp Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Dry Cal check
#1-3

pre calibration
adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/19/2026 14:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:48
02 Std. Gas	0.077	14:49
03 Room Air	0.000	14:49
04 Std. Gas	0.077	14:49
05 Room Air	0.000	14:50
06 Std. Gas	0.077	14:50
07 Room Air	0.000	14:51

Lot No = 19825080A2
Cyl No = 23
Exp Date = 09/05/2027
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Dry cal check pre calibration
#4-6 adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/25/2026 08:53

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:54
02 Std. Sol.	0.024	08:55
03 Room Air	0.000	08:55
04 Std. Sol.	0.024	08:56
05 Room Air	0.000	08:57
06 Std. Sol.	0.023	08:57
07 Room Air	0.000	08:58

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202509A
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Low AC check
0.025AC

post calibration
adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/25/2026 09:04

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:04
02 Std. Sol.	0.392	09:06
03 Room Air	0.000	09:06
04 Std. Sol.	0.394	09:07
05 Room Air	0.000	09:08
06 Std. Sol.	0.393	09:08
07 Room Air	0.000	09:09

08 Sim Temp = 34.0°C

Simul Ser No = MP3065
Std Sol No = 202506H
County = 08 Oper No. = 133237


Operator Signature
ANNA INGEMANSEN

Remarks:

High AC check
0.400AC

post calibration
adjustment.

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/25/2026 09:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:15
02 Std. Gas	0.079	09:15
03 Room Air	0.000	09:16
04 Std. Gas	0.079	09:16
05 Room Air	0.000	09:17
06 Std. Gas	0.079	09:17
07 Room Air	0.000	09:18

Lot No = 264437
Cyl No = 114
Exp Date = 01/29/2028
County = 08 Oper No. = 133237

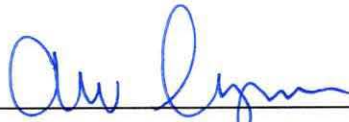

Operator Signature
ANNA INGEMANSEN

Remarks:

dry cal check
#1-3

Post calibration
adjustment.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/25/2026 09:18

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:18
02 Std. Gas	0.079	09:19
03 Room Air	0.000	09:19
04 Std. Gas	0.079	09:20
05 Room Air	0.000	09:20
06 Std. Gas	0.080	09:21
07 Room Air	0.000	09:21


Lot No = 264437

Cyl No = 114

Exp Date = 01/29/2028

County = 08

Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Dry cal check
#4-6

post calibration
adjustment.

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = TOXL 8164.14.00 09/16
06/25/2026 09:22

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:22
02 Std. Gas	0.079	09:23
03 Room Air	0.000	09:23
04 Std. Gas	0.080	09:23
05 Room Air	0.000	09:24
06 Std. Gas	0.080	09:24
07 Room Air	0.000	09:25

Lot No = 264437
Cyl No = 114
Exp Date = 01/29/2028
County = 08 Oper No. = 133237



Operator Signature
ANNA INGEMANSEN

Remarks:

Dry cal check
#7-9

post calibration
adjustment.

Form 106-I8000