



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
SFN 59281 (06/2018)

Serial Number <u>80-005943</u>	Instrument Location <u>City of Lakota Courthouse Nelson County</u>
Reason for Install/Repair ☐ Install After Receiving From Crime Laboratory ☐ Install After Location Change ☒ Other (Specify) <u>Install after Receiving from Crime Laboratory Annual Inspection</u>	

Check When Done:

- ☒ 1. Surge Protector Installed/Property Grounded.
- ☒ 2. Telephone Line Connected to Intoxilyzer® 8000.
- ☒ 3. Breath Tube Heated.
- ☒ 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- ☒ 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).

AEI ☒ 6. Run Tests:

- 7/7/26
- ☒ A. Print Test (Level 1, Function P).
 - ☒ B. ACA Test (Level 1, Function C).
 - ☒ C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
 - ☒ 7. Repair and/or Maintenance Performed (if any): Annual Maintenance 5-24-26
 - ☒ 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
 - ☒ 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
 - ☒ 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <u>[Signature]</u> #4480	Date <u>6-25-26</u>
---	------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <u>Anna Ingemansen</u> <u>Ann Ingemansen</u>	Certified Date <u>07Jul2026</u>
---	------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005943
Location = NCSO 8164.14.00 09/16
06/25/2026 11:09

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup

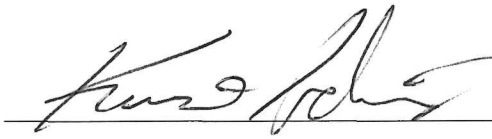
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.085
Standard Lot #? 19825080A2
Standard Cyl #? 28
Standard Expiration? 09/05/2027
Oper No? 132972

Flow Cal. Date: 06/20/2013
Slope 686
Intercept -735246

IR Calibration Date: 08/26/2016
 3um 9um

0th Coef(*100):	-13589	-19547
1st Coef(*100):	284566	139614
2nd Coef(*100):	2717	1336
H2O adj(mg/l*10k):	381	404

***** Printer Test End *****

 #4480
Operator Signature
KURT SCHWIND

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005943
Location = NCSO 8164.14.00 09/16
06/25/2026 11:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:11
02 Std. Gas	0.078	11:11
03 Room Air	0.000	11:12
04 Std. Gas	0.079	11:12
05 Room Air	0.000	11:13
06 Std. Gas	0.079	11:13
07 Room Air	0.000	11:13

Lot No = 19825080A2
Cyl No = 28
Exp Date = 09/05/2027
County = 32 Oper No. = 132972

 #4480

Operator Signature
KURT SCHWIND

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005943
Location = NCSO 8164.14.00 09/16
06/25/2026 11:33

Test	AC	Time
01 Room Air	0.000	11:35
02 *Subject Test	RFI*	11:36
03 Room Air	0.000	11:36

*Invalid Test
Inhibited - RFI

Sub Name = SCHWIND, KURT DOUGLAS
Sub DOB = 07/01/1967
Sub Sex = Male Weight = 200
Test = OTH Cit = 0000000
Dr. Lic. = ND/SCH675792
Lot No = 19825080A2
Cyl No = 28
Expiration Date = 09/05/2027
County = 32 Oper No. = 132972

 #4480

Operator Signature
KURT SCHWIND

Remarks:

Form 106-I8000