



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
SFN 59281 (06/2018)

Serial Number 80-005362	Instrument Location BIA Spirit Lake Police
Reason for Install/Repair ☐ Install After Receiving From Crime Laboratory ☐ Install After Location Change ☒ Other (Specify) <u>re-install at same location, running all Cal test on same date</u>	

Check When Done:


- ☒ 1. Surge Protector Installed/Property Grounded.
☐ 2. Telephone Line Connected to Intoxilyzer® 8000.
☒ 3. Breath Tube Heated.
☒ 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
☒ 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
☒ 6. Run Tests:
 ☒ A. Print Test (Level 1, Function P).
 ☒ B. ACA Test (Level 1, Function C).
 ☒ C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
☐ 7. Repair and/or Maintenance Performed (if any): N/A
☒ 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
☐ 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
☒ 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

AEI
25Sep26

Field Inspector Signature 	Date 9/6/26
--	----------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By Anna Ingemansen		Certified Date 25Sep2026
--	--	-----------------------------

Anna Ingemansen checked off #6 as all three tests were run. This does not affect the installation of this instrument. AEI 25Sep26

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = FTOT 8164.14.00 09/16
09/06/2026 13:19

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 264437
Standard Cyl #? 110
Standard Expiration? 01/29/2028
Oper No? 133407

Flow Cal. Date: 05/22/2020
Slope 659
Intercept -620990

IR Calibration Date: 06/05/2025
 3um 9um

0th Coef(*100):	-17586	-20811
1st Coef(*100):	258173	138666
2nd Coef(*100):	3503	1716
H2O adj(mg/l*10k):	416	438

***** Printer Test End *****

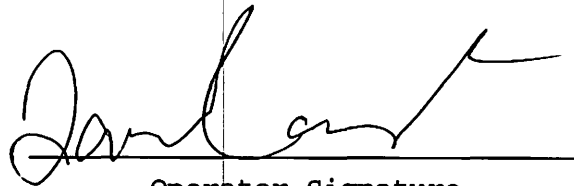

Operator Signature
TARA CAVANAUGH

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = FTOT 8164.14.00 09/16
09/06/2026 13:04

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:05
02 Std. Gas	<u>0.078</u>	13:05
03 Room Air	0.000	13:06
04 Std. Gas	<u>0.079</u>	13:06
05 Room Air	0.000	13:07
06 Std. Gas	<u>0.079</u>	13:07
07 Room Air	0.000	13:08


Lot No = 264437

Cyl No = 110

Exp Date = 01/29/2028

County = 62

Oper No. = 133407

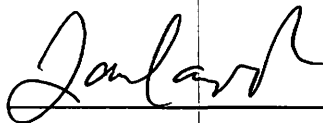

Operator Signature
TARA CAVANAUGH

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005362
Location = FTOT 8164.14.00 09/16
09/06/2026 13:23

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:24
02 Std. Gas	0.078	13:24
03 Room Air	0.000	13:25
04 Std. Gas	RFI*	13:25
05 Room Air	0.000	13:26

*Invalid Test
Inhibited - RFI

Lot No = 264437
Cyl No = 110
Exp Date = 01/29/2028
County = 62 Oper No. = 133407

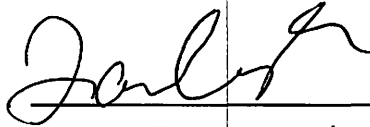

Operator Signature
TARA CAVANAUGH

Remarks:

Form 106-I8000