



ETHANOL GAS STANDARD CYLINDER REPORT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59282 (08/2018)

Chemical Test Operator Name (Print) ANTHONY HILL		
Location ROLLA (40)		Intoxilyzer® Serial Number 80-004204
Gas Lot Number 264944	Gas Cylinder Number 307	Gas Expiration Date 5/12/2028

Check When Done:

☒ 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).

☒ 2. Perform an ACA Test (Level 1, Function C).

Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).

A. 0. **80** AC

B. 0. **80** AC

C. 0. **80** AC



☒ 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.

☒ 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.

☒ 5. Send the Following to the Crime Laboratory:

A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).

B. ACA Test Record.

Chemical Test Operator Signature 	Date 9/27/26
Reviewed By (Crime Laboratory Use Only) Anna Ingemansen 	Date 30Sept2026

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004204
Location = ROLL 8164.14.00 09/16
09/27/2026 03:23

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	03:24
02 Std. Gas	0.081	03:24
03 Room Air	0.000	03:25
04 Std. Gas	0.080	03:25
05 Room Air	0.000	03:26
06 Std. Gas	0.080	03:26
07 Room Air	0.000	03:26

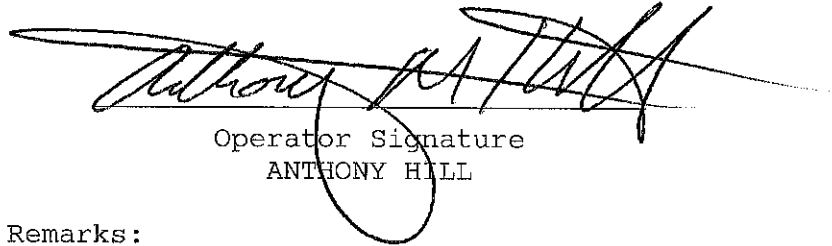
Lot No = 264944

Cyl No = 307

Exp Date = 05/12/2028

County = 40

Oper No. = 133866



Operator Signature
ANTHONY HILL

Remarks:

Form 106-I8000